

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100523\
 Data File : VW032266.D
 Acq On : 05 Oct 2023 19:25
 Operator : SY/MD
 Sample : 04748-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EO5K2

Quant Time: Oct 06 01:32:11 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 06 01:20:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	87088	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	93045	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	42653	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	28738	4.057	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.200%
7) Chloroethane-d5	1.532	69	26713	4.646	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.000%
11) 1,1-Dichloroethene-d2	2.059	65	12026	4.026	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.600%
20) 2-Butanone-d5	3.799	46	84104	46.941	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.880%
24) Chloroform-d	4.256	84	56424	4.516	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.400%
26) 1,2-Dichloroethane-d4	4.947	65	28567	4.827	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.600%
32) Benzene-d6	4.963	84	109579	4.002	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.000%
36) 1,2-Dichloropropane-d6	5.992	67	37307	4.113	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	82.200%
41) Toluene-d8	7.249	98	98186	3.922	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.400%
43) trans-1,3-Dichloroprop...	7.564	79	12526	3.897	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.000%
46) 2-Hexanone-d5	8.030	63	62295	41.190	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.380%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	26719	4.211	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.200%
66) 1,2-Dichlorobenzene-d4	11.564	152	37701	4.763	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.200%
Target Compounds						Qvalue
13) Acetone	2.133	43	2723	1.972	ug/L	84
34) Trichloroethene	5.847	95	1663	0.186	ug/L	# 78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032266.D
Acq On : 05 Oct 2023 19:25
Operator : SY/MD
Sample : 04748-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EO5K2

Quant Time: Oct 06 01:32:11 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 06 01:20:04 2023
Response via : Initial Calibration

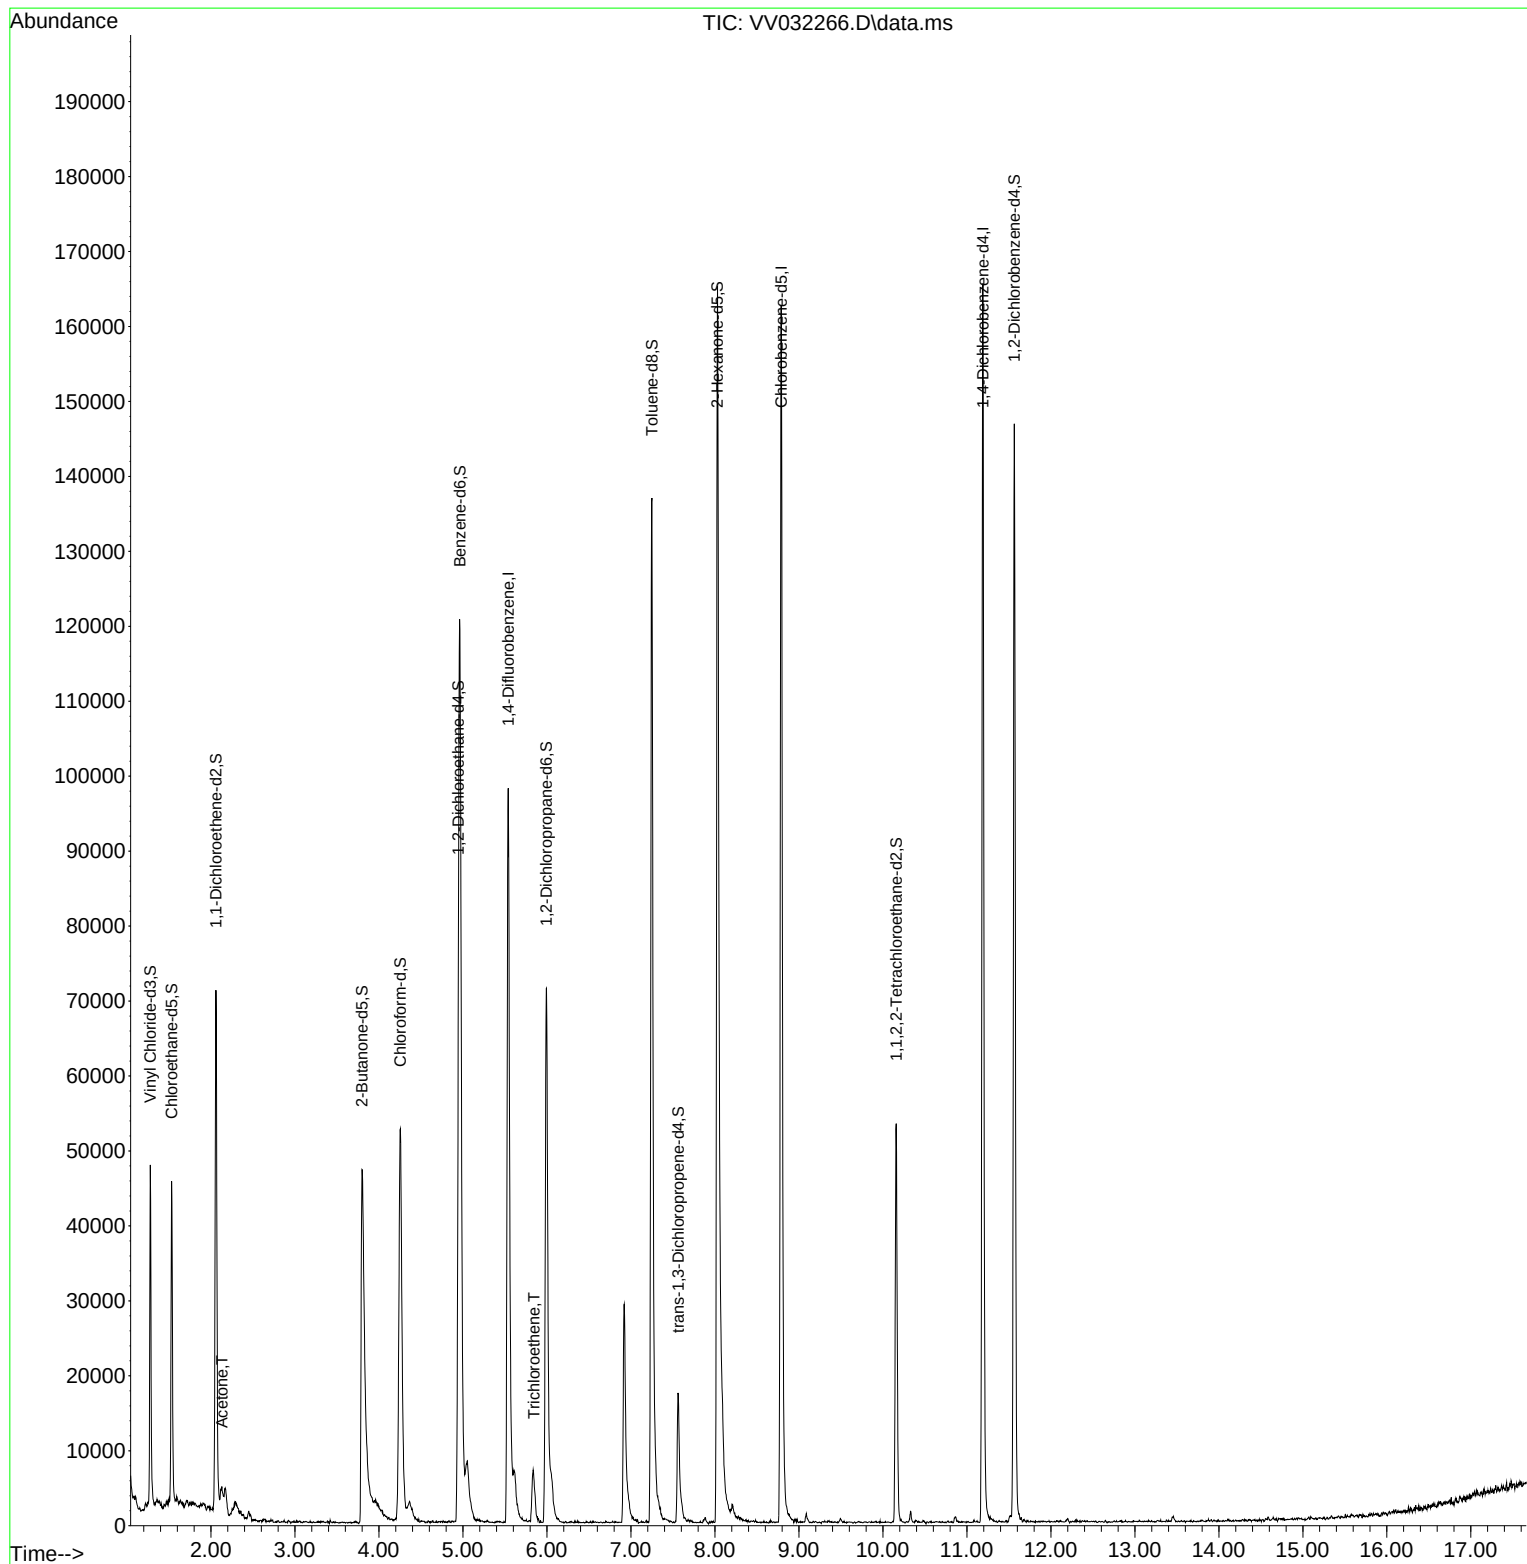

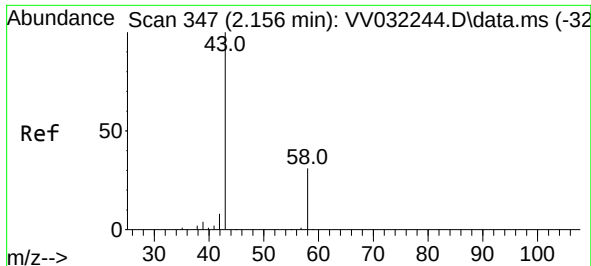

#13

Acetone

Concen: 1.972 ug/L

RT: 2.133 min Scan# 34

Delta R.T. -0.023 min

Lab File: VV032266.D

Acq: 05 Oct 2023 19:25

Instrument :

MSVOA_V

ClientSampleId :





EO5K2

Tgt Ion: 43 Resp: 2723

Ion Ratio Lower Upper

43 100

58 24.2 0.0 66.0

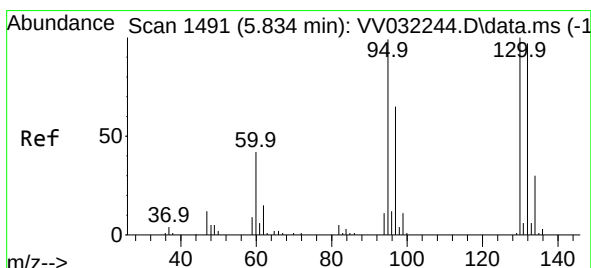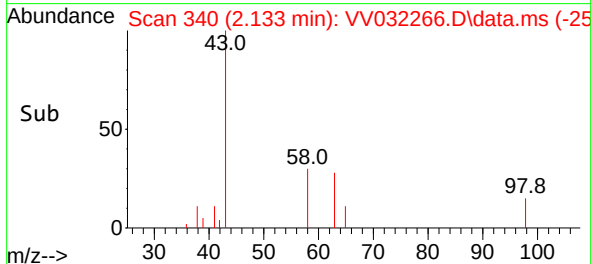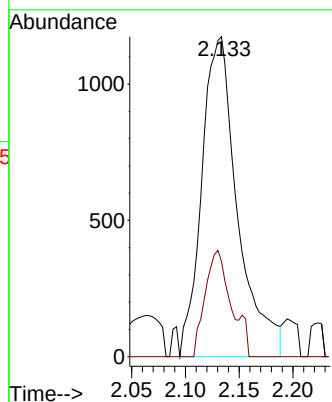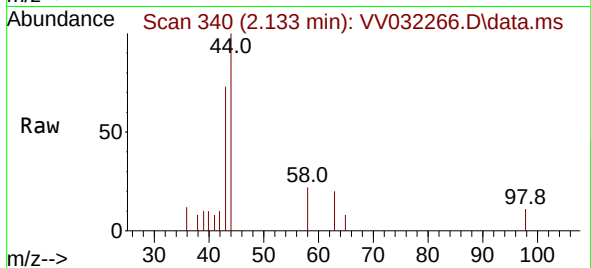

#34

Trichloroethene

Concen: 0.186 ug/L

RT: 5.847 min Scan# 1495

Delta R.T. 0.013 min

Lab File: VV032266.D

Acq: 05 Oct 2023 19:25

Tgt Ion: 95 Resp: 1663

Ion Ratio Lower Upper

95 100

97 50.1 45.7 84.9

132 69.9 70.3 130.5

130 84.3 69.6 129.2

