

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100523\
 Data File : VW032272.D
 Acq On : 05 Oct 2023 22:12
 Operator : SY/MD
 Sample : 04741-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ5

Quant Time: Oct 06 05:26:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 06 05:25:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	86131	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	90359	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	41378	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	26051	3.719	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.400%
7) Chloroethane-d5	1.532	69	25329	4.455	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.000%
11) 1,1-Dichloroethene-d2	2.056	65	11276	3.817	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.400%
20) 2-Butanone-d5	3.825	46	84057	47.436	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.880%
24) Chloroform-d	4.252	84	54797	4.434	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.600%
26) 1,2-Dichloroethane-d4	4.947	65	26862	4.589	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.800%
32) Benzene-d6	4.963	84	104026	3.913	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	78.200%
36) 1,2-Dichloropropane-d6	5.992	67	38087	4.324	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.400%
41) Toluene-d8	7.249	98	91717	3.772	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.400%
43) trans-1,3-Dichloroprop...	7.561	79	11676	3.740	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.800%
46) 2-Hexanone-d5	8.034	63	60359	41.096	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.200%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	27445	4.454	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.000%
66) 1,2-Dichlorobenzene-d4	11.564	152	35002	4.559	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.200%
Target Compounds						Qvalue
47) Tetrachloroethene	7.915	164	4380	0.665	ug/L	96
49) Dibromochloromethane	8.185	129	2562	0.410	ug/L	82
59) Bromoform	9.677	173	535	0.178	ug/L #	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032272.D
Acq On : 05 Oct 2023 22:12
Operator : SY/MD
Sample : 04741-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ5

Quant Time: Oct 06 05:26:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 06 05:25:10 2023
Response via : Initial Calibration

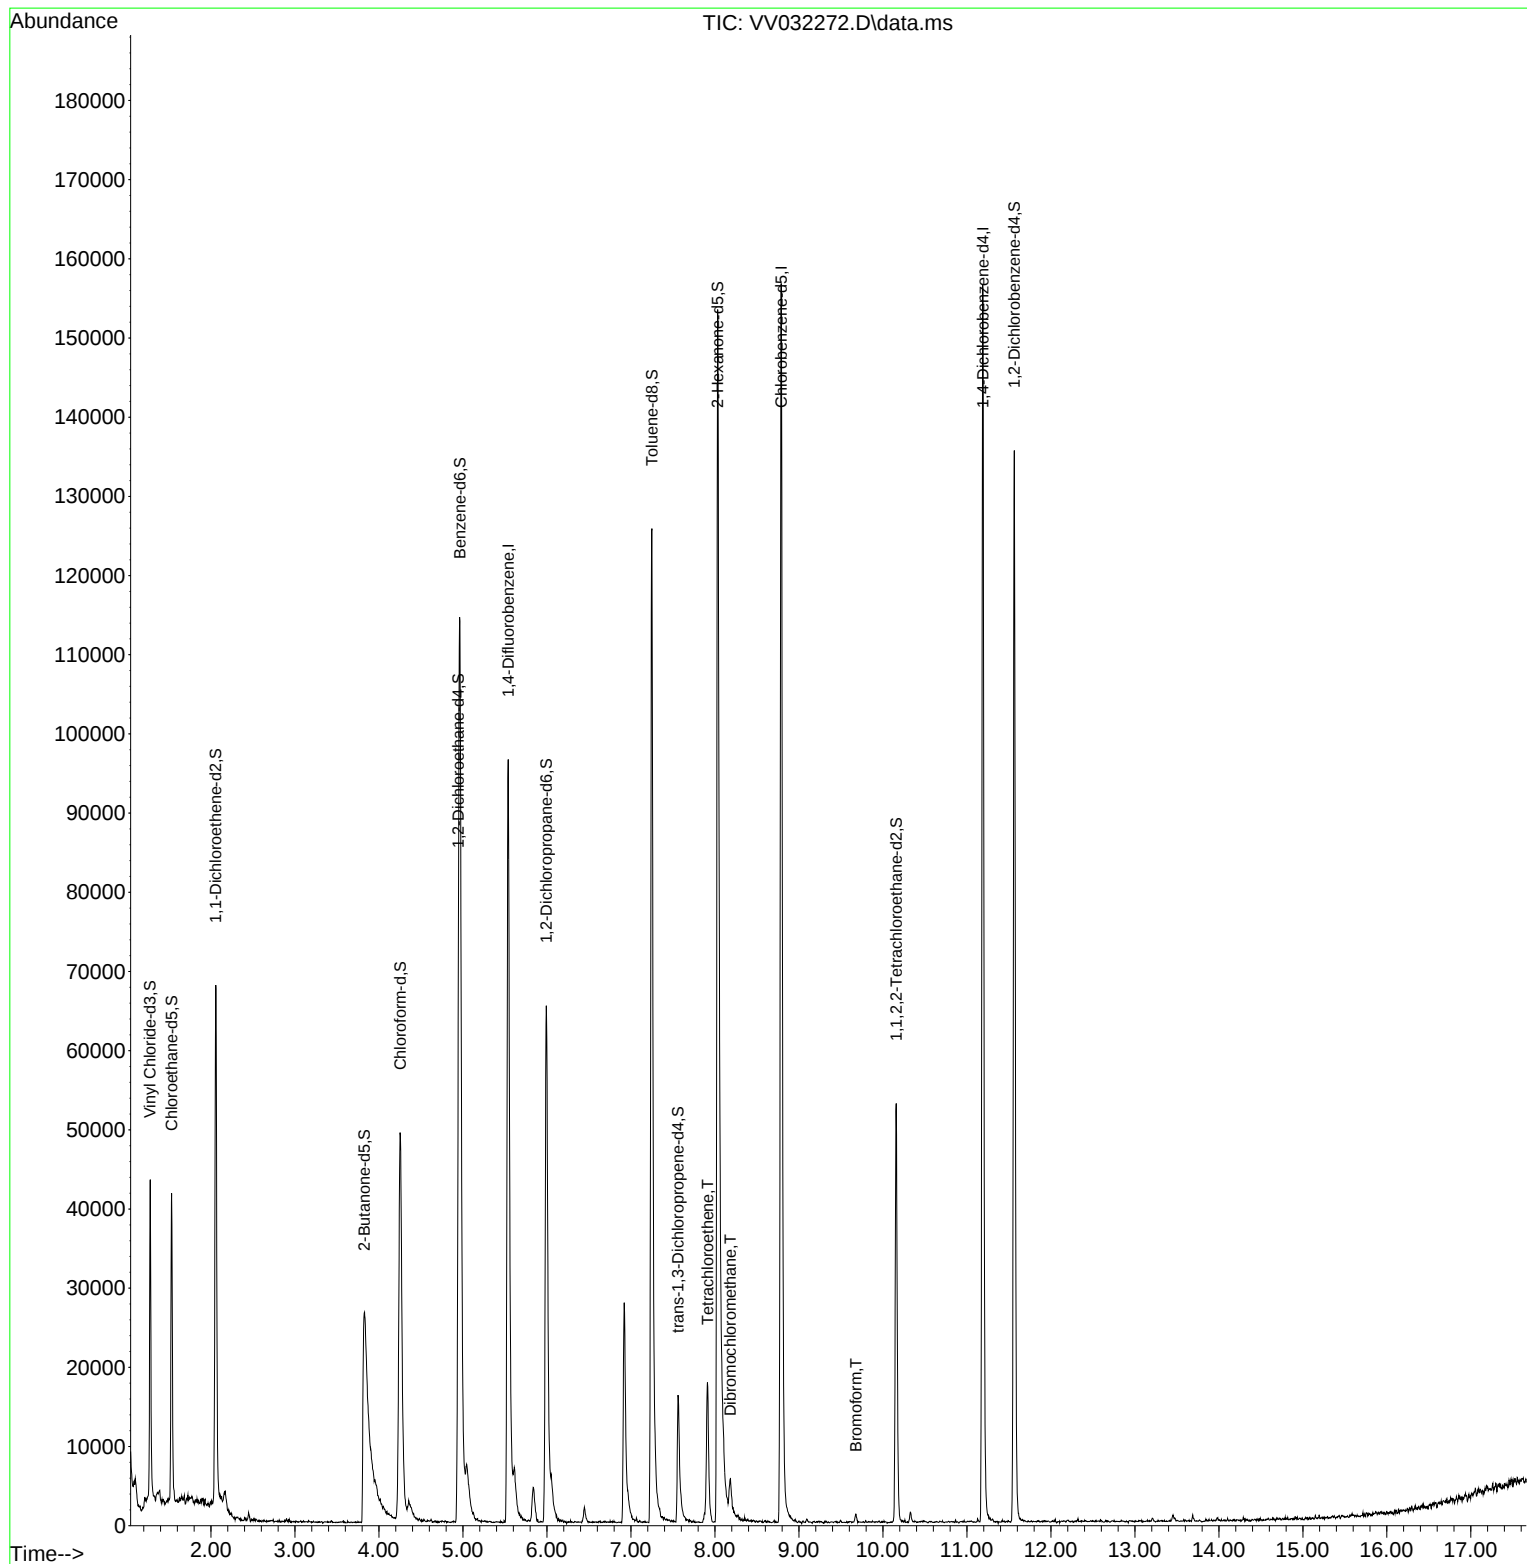

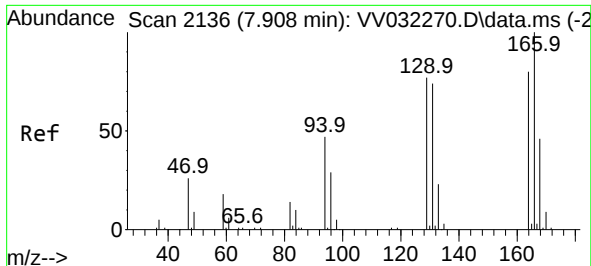

#47

Tetrachloroethene

Concen: 0.665 ug/L

RT: 7.915 min Scan# 2136

Delta R.T. 0.006 min

Lab File: VV032272.D

Acq: 05 Oct 2023 22:12

Instrument :

MSVOA_V

ClientSampleId :

C0AZ5

Tgt Ion:164 Resp: 4380





Ion Ratio Lower Upper

164 100

129 98.3 66.4 123.4

131 91.1 63.7 118.3

166 117.8 87.9 163.3

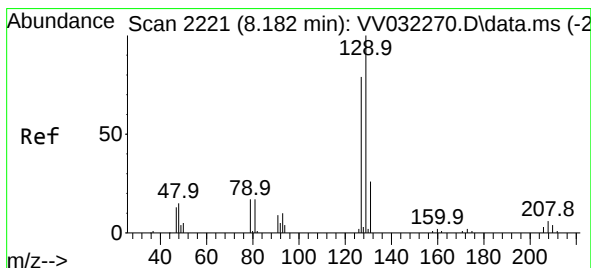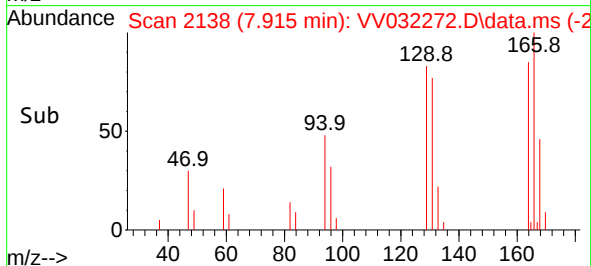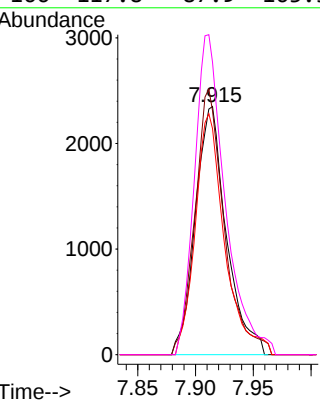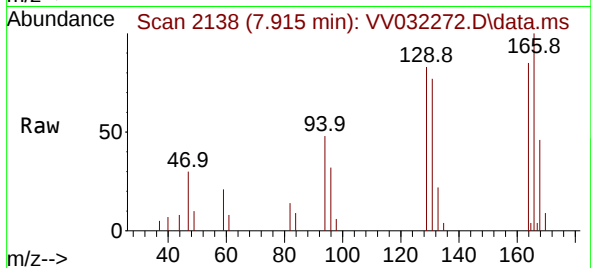

#49

Dibromochloromethane

Concen: 0.410 ug/L

RT: 8.185 min Scan# 2222

Delta R.T. 0.003 min

Lab File: VV032272.D




Acq: 05 Oct 2023 22:12


Tgt Ion:129 Resp: 2562

Ion Ratio Lower Upper

129 100

127 65.6 57.2 106.2

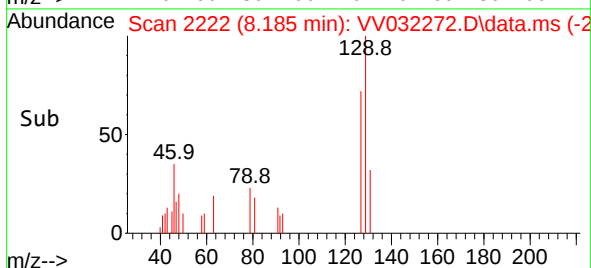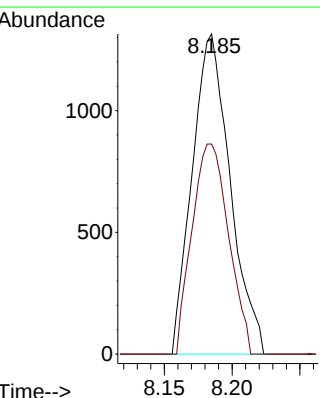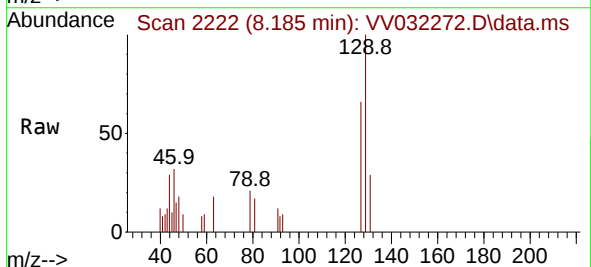

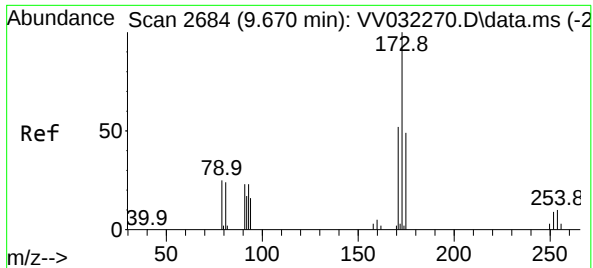

#59
 Bromoform
 Concen: 0.178 ug/L
 RT: 9.677 min Scan# 2
 Delta R.T. 0.006 min
 Lab File: VV032272.D
 Acq: 05 Oct 2023 22:12

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ5

Tgt Ion:173 Resp: 535
 Ion Ratio Lower Upper
 173 100
 175 43.2 38.2 57.2
 254 0.0 7.0 10.4#

