

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
 Data File : VV032248.D
 Acq On : 05 Oct 2023 12:08
 Operator : SY/MD
 Sample : 04741-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B00

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032248.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	85	rBV	49106	51743	14.45%	1.823%
2	1.355	93	98	110	rVB2	2625	4185	1.17%	0.147%
3	1.532	146	153	165	rVB	45468	53540	14.95%	1.886%
4	2.059	308	317	330	rBV	80708	117679	32.86%	4.146%
5	3.821	854	865	903	rBV	29522	129495	36.16%	4.562%
6	4.252	984	999	1024	rBV2	54648	144211	40.27%	5.081%
7	4.963	1205	1220	1241	rBV2	131158	336938	94.10%	11.870%
8	5.538	1387	1399	1437	rBV	99698	218047	60.89%	7.682%
9	5.831	1481	1490	1509	rVB3	4235	9448	2.64%	0.333%
10	5.992	1527	1540	1577	rBV	76860	170360	47.58%	6.002%
11	6.921	1818	1829	1860	rBV	32758	69732	19.47%	2.457%
12	7.249	1920	1931	1957	rBV	147231	275475	76.93%	9.705%
13	7.561	2017	2028	2046	rBV2	18569	37086	10.36%	1.307%
14	8.034	2165	2175	2216	rBV2	148847	358076	100.00%	12.615%
15	8.789	2398	2410	2432	rBV	161824	273933	76.50%	9.651%
16	10.159	2826	2836	2861	rVB	54338	87845	24.53%	3.095%
17	10.329	2879	2889	2898	rVB2	3332	4731	1.32%	0.167%
18	11.188	3146	3156	3179	rBV	159807	255230	71.28%	8.992%
19	11.564	3262	3273	3295	rBV	151895	240710	67.22%	8.480%




Sum of corrected areas: 2838464

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032248.D
Acq On : 05 Oct 2023 12:08
Operator : SY/MD
Sample : 04741-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

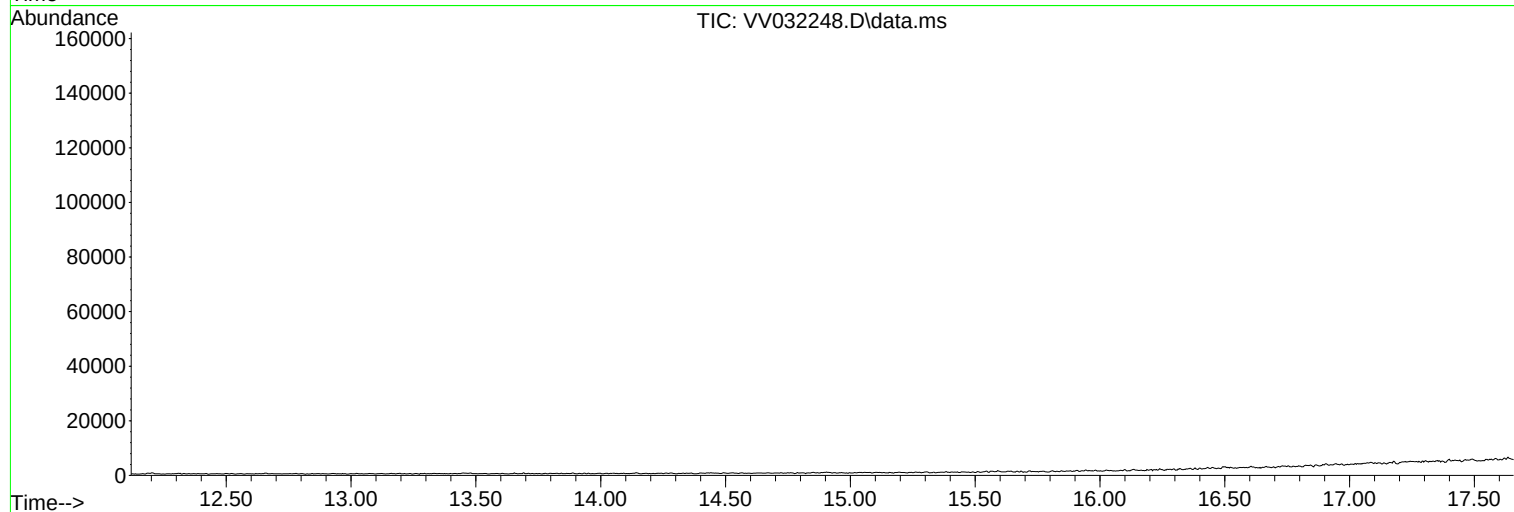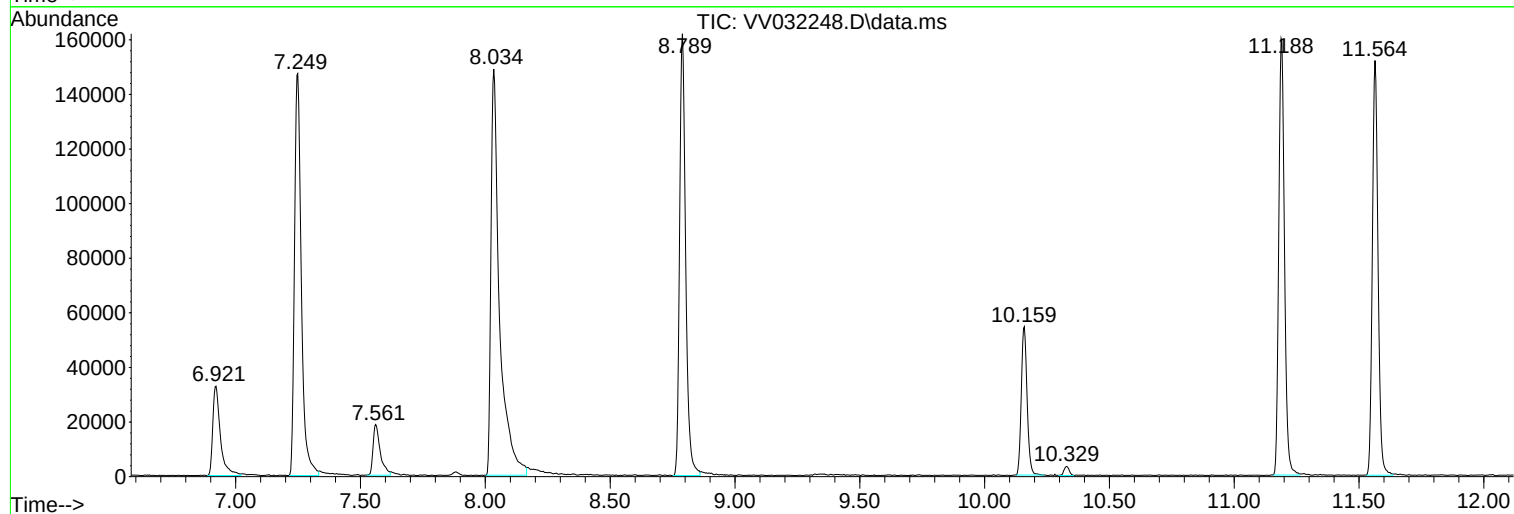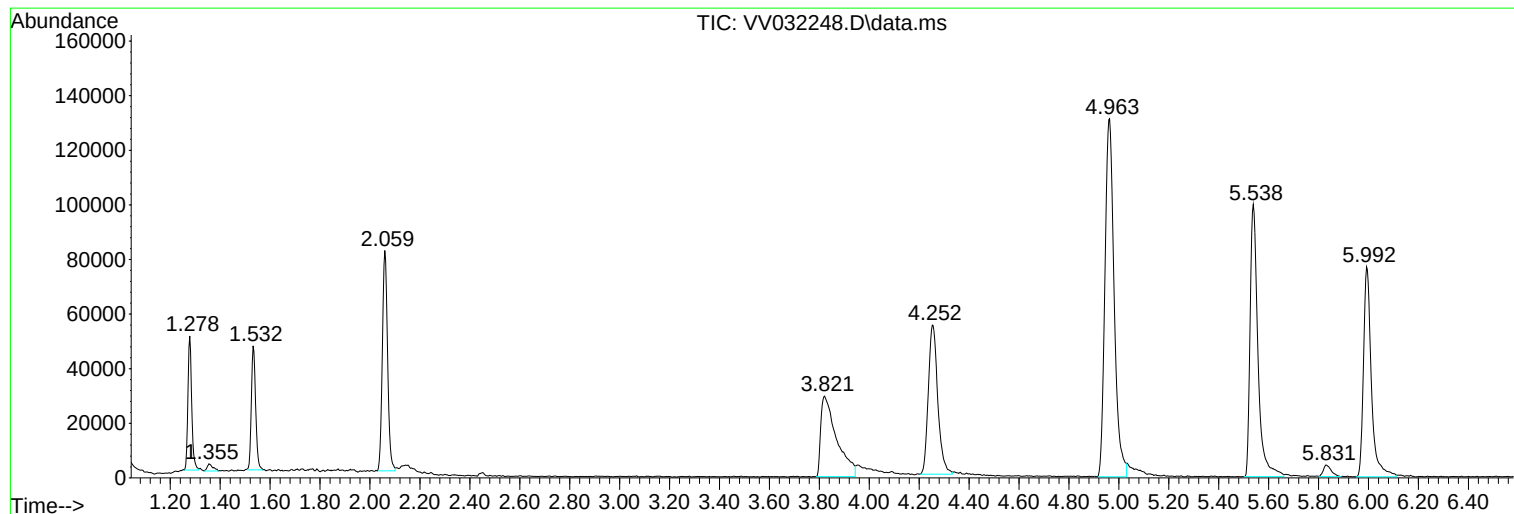

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032248.D
Acq On : 05 Oct 2023 12:08
Operator : SY/MD
Sample : 04741-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032248.D
Acq On : 05 Oct 2023 12:08
Operator : SY/MD
Sample : 04741-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc