

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
 Data File : VV032250.D
 Acq On : 05 Oct 2023 12:55
 Operator : SY/MD
 Sample : 04744-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH578

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032250.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.532	146	153	166	rBV	45107	52120	14.23%	1.792%
2	2.060	307	317	332	rBV	49694	73793	20.15%	2.538%
3	3.812	852	862	905	rBV2	40762	144368	39.42%	4.965%
4	4.259	984	1001	1033	rBV3	61808	201061	54.90%	6.914%
5	4.963	1204	1220	1242	rBV2	129150	332565	90.81%	11.437%
6	5.539	1387	1399	1423	rBV	112615	241443	65.93%	8.303%
7	5.834	1482	1491	1502	rBV4	3749	7762	2.12%	0.267%
8	5.995	1528	1541	1560	rBV	76471	165200	45.11%	5.681%
9	6.442	1668	1680	1700	rBV2	14834	30807	8.41%	1.059%
10	6.921	1818	1829	1848	rBV	22885	47085	12.86%	1.619%
11	7.249	1921	1931	1962	rBV	55514	105254	28.74%	3.620%
12	7.561	2020	2028	2043	rBV	13818	25978	7.09%	0.893%
13	8.034	2162	2175	2208	rBV	171467	366213	100.00%	12.594%
14	8.182	2212	2221	2239	rVB3	10329	21230	5.80%	0.730%
15	8.789	2397	2410	2437	rBV	181371	312001	85.20%	10.729%
16	10.156	2825	2835	2853	rBV	58280	93631	25.57%	3.220%
17	10.310	2872	2883	2901	rBV	56167	91008	24.85%	3.130%
18	10.429	2912	2920	2941	rVB2	20866	33773	9.22%	1.161%
19	11.188	3145	3156	3181	rBV	188094	294557	80.43%	10.129%
20	11.487	3241	3249	3262	rBV2	5414	8079	2.21%	0.278%
21	11.564	3262	3273	3303	rVV	154406	259997	71.00%	8.941%




Sum of corrected areas: 2907925

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032250.D
Acq On : 05 Oct 2023 12:55
Operator : SY/MD
Sample : 04744-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH578

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

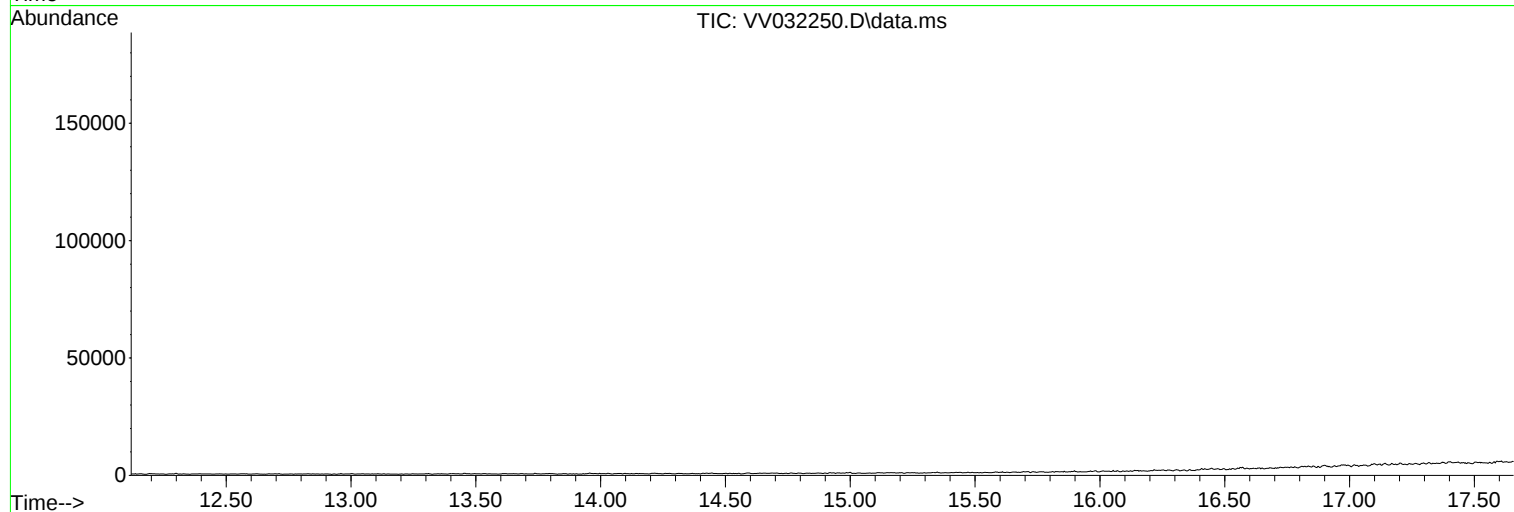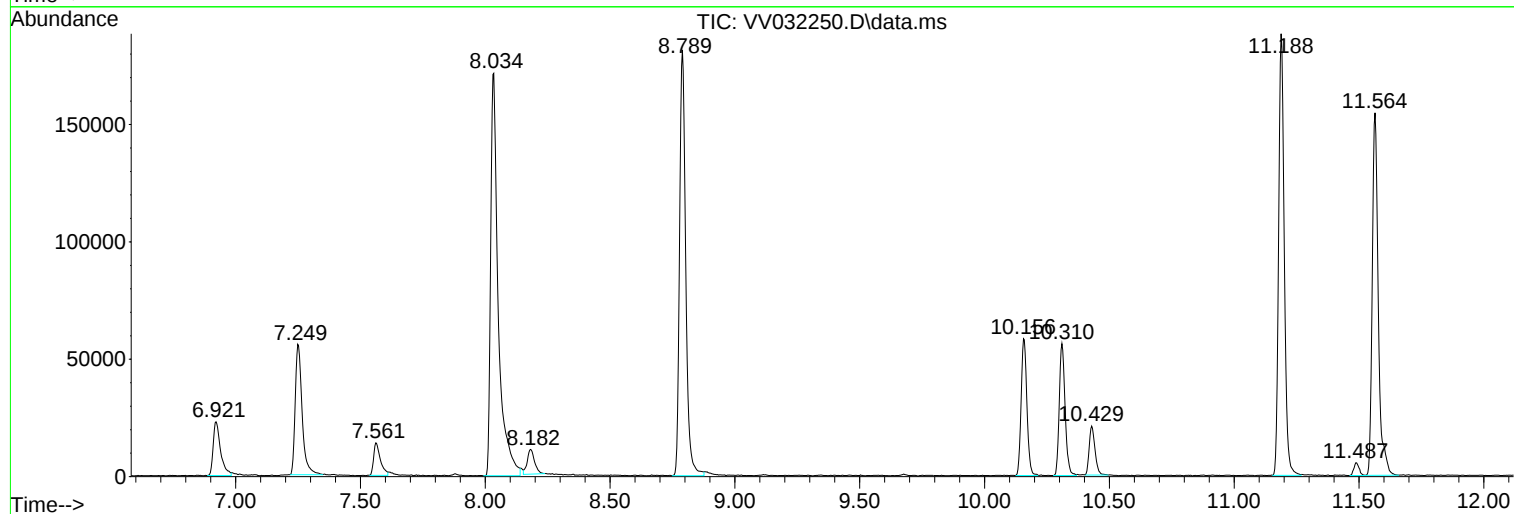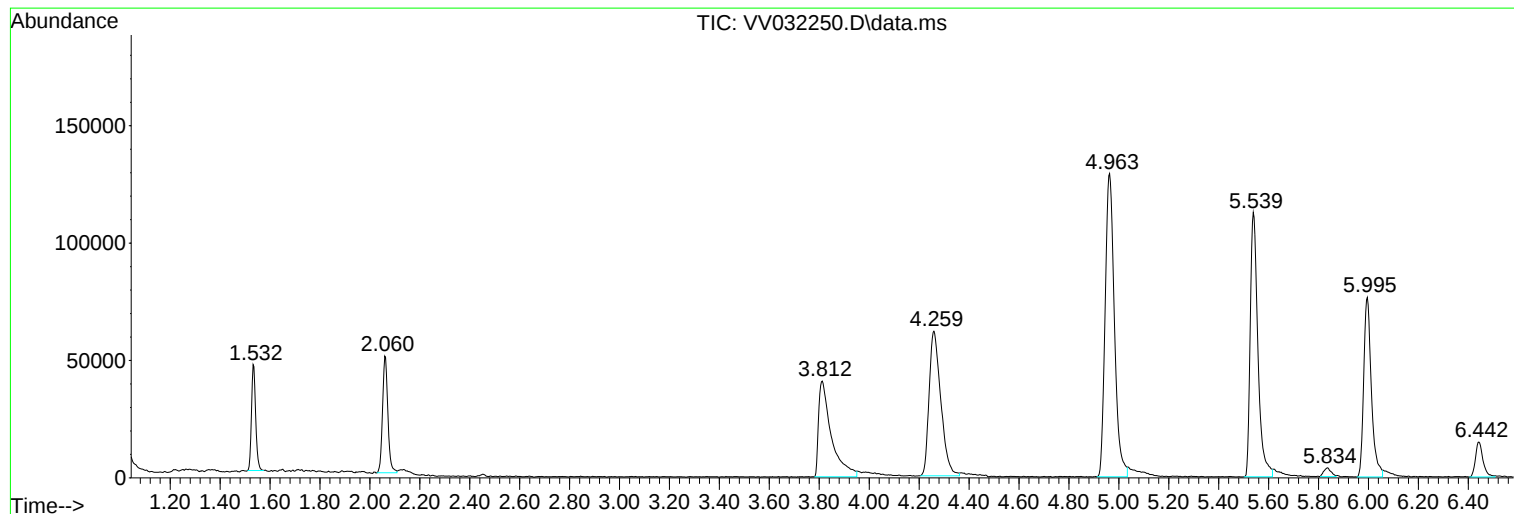

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032250.D
Acq On : 05 Oct 2023 12:55
Operator : SY/MD
Sample : 04744-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH578










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.310	1.54 ug/L	91008	1,4-Dichlorobenzene-d4	11.188

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Chloro-N-(1,1-dioxidotetrahydr...	225	C7H12ClNO3S	007365-23-3	45
2			Encainide	352	C22H28N2O2	037612-13-8	43
3			Benzen-d5-amine	98	C6H2D5N	004165-61-1	32
4			Acetonitrile, isothiocyanato-	98	C3H2N2S	032772-75-1	32
5			Phenyl-piperidin-1-ylmethyl-phos...	281	C15H24NO2P	1000294-47-8	32

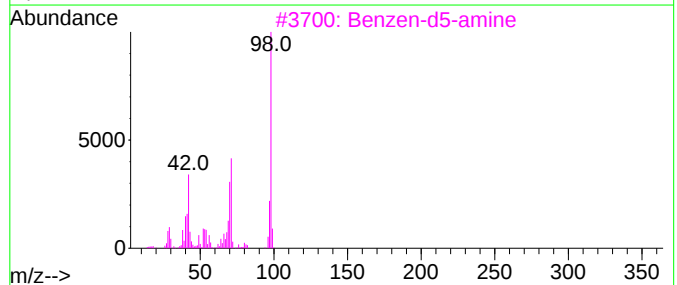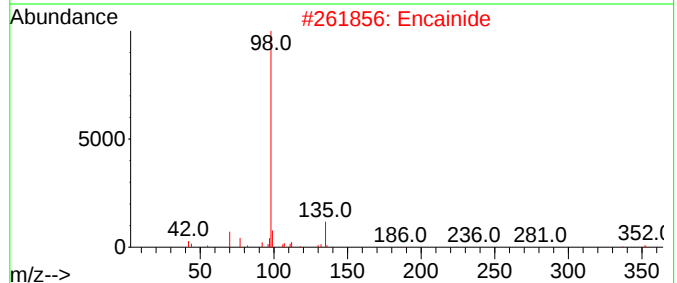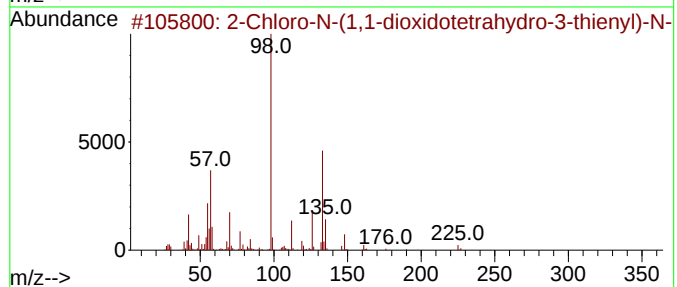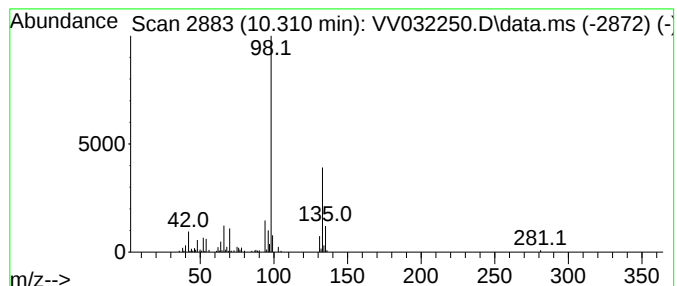

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032250.D
Acq On : 05 Oct 2023 12:55
Operator : SY/MD
Sample : 04744-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH578










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown-02 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.429	0.57 ug/L	33773	1,4-Dichlorobenzene-d4	11.188

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Eperisone	259	C17H25NO	064840-90-0	45
2			Benzen-d5-amine	98	C6H2D5N	004165-61-1	37
3			Acetonitrile, isothiocyanato-	98	C3H2N2S	032772-75-1	32
4			Encainide	352	C22H28N2O2	037612-13-8	32
5			2-Benzyl-1-methylpiperidine	189	C13H19N	031414-56-9	25

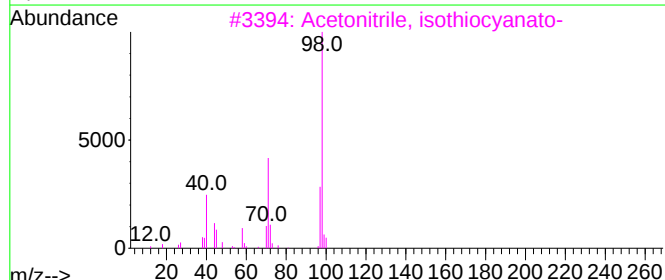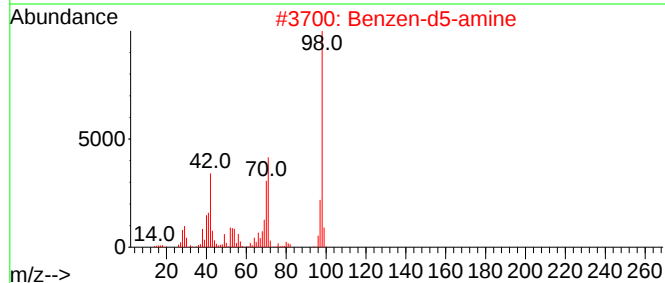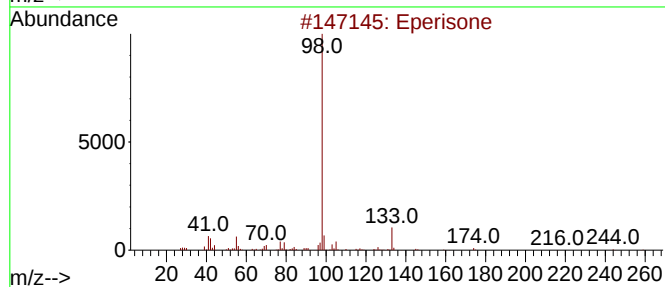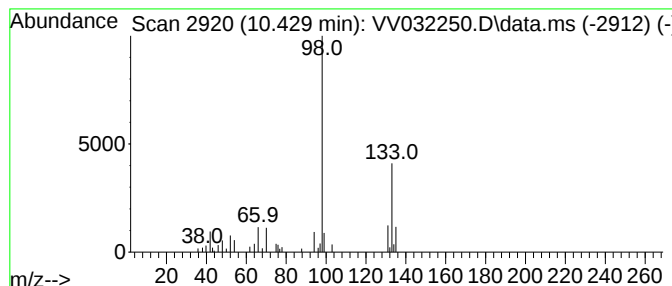

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032250.D
Acq On : 05 Oct 2023 12:55
Operator : SY/MD
Sample : 04744-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH578

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	10.310	1.5	ug/L	91008	3	11.188	294557	5.0
unknown-02	10.429	0.6	ug/L	33773	3	11.188	294557	5.0