

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
 Data File : VV032252.D
 Acq On : 05 Oct 2023 13:43
 Operator : SY/MD
 Sample : 04744-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH580

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032252.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.532	145	153	164	rBV	89711	105029	13.82%	1.818%
2	2.060	307	317	330	rBV	100713	146223	19.24%	2.531%
3	3.796	846	857	899	rBV	97681	300605	39.56%	5.204%
4	4.256	983	1000	1031	rBV3	123502	389699	51.29%	6.747%
5	4.960	1200	1219	1246	rBV2	261183	679992	89.49%	11.772%
6	5.535	1386	1398	1435	rBV	207205	442697	58.26%	7.664%
7	5.828	1479	1489	1510	rBV2	7372	16274	2.14%	0.282%
8	5.992	1523	1540	1569	rBV	155238	337102	44.37%	5.836%
9	6.439	1666	1679	1697	rBV2	24604	50019	6.58%	0.866%
10	6.918	1817	1828	1861	rBV2	46135	93355	12.29%	1.616%
11	7.249	1919	1931	1951	rBV	104958	189293	24.91%	3.277%
12	7.561	2016	2028	2046	rBV	28733	56024	7.37%	0.970%
13	8.027	2162	2173	2211	rBV	386842	759830	100.00%	13.154%
14	8.182	2212	2221	2240	rVB2	15193	32559	4.29%	0.564%
15	8.789	2398	2410	2435	rBV	326014	554851	73.02%	9.606%
16	10.156	2823	2835	2858	rBV	118690	188860	24.86%	3.270%
17	10.310	2870	2883	2901	rBV	148948	242683	31.94%	4.201%
18	10.426	2910	2919	2942	rVB	61534	98054	12.90%	1.698%
19	11.188	3145	3156	3176	rBV	353646	543352	71.51%	9.407%
20	11.490	3241	3250	3261	rBV2	10411	15912	2.09%	0.275%
21	11.564	3261	3273	3297	rBV	316774	533812	70.25%	9.242%




Sum of corrected areas: 5776225

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032252.D
Acq On : 05 Oct 2023 13:43
Operator : SY/MD
Sample : 04744-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH580

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

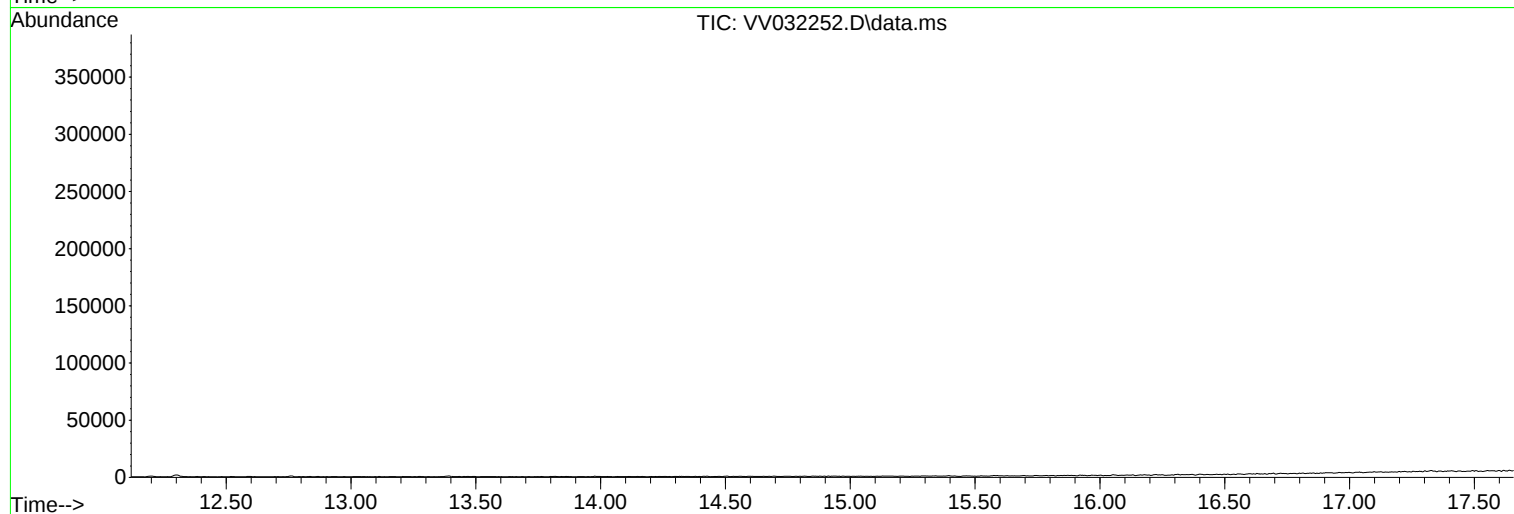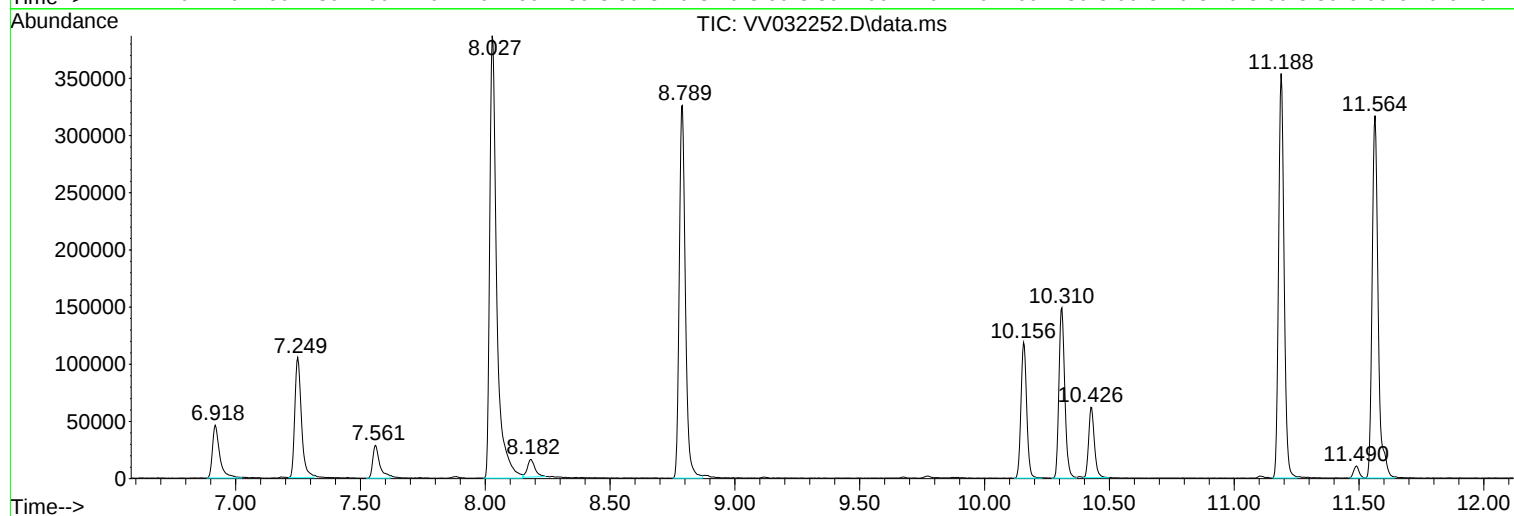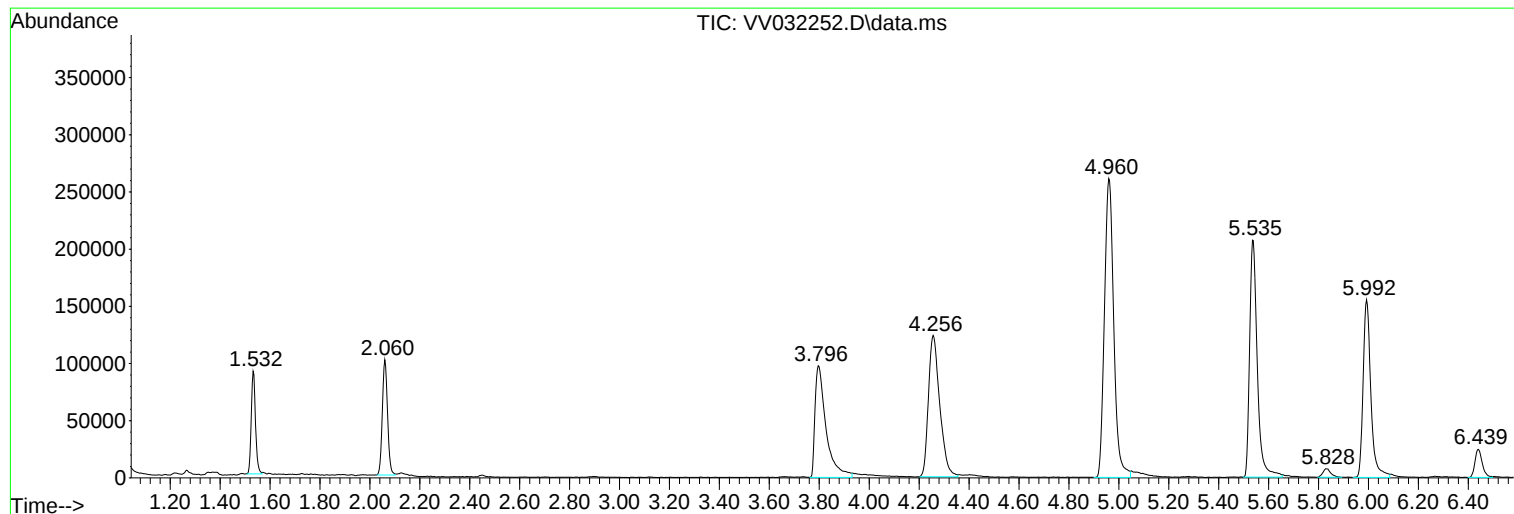

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032252.D
Acq On : 05 Oct 2023 13:43
Operator : SY/MD
Sample : 04744-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH580










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.310	2.23 ug/L	242683	1,4-Dichlorobenzene-d4	11.188

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Mepivacaine	246	C15H22N2O	000096-88-8	47
2			Piperidine, 4-chloro-1-methyl-	133	C6H12ClN	005570-77-4	45
3			Encainide	352	C22H28N2O2	037612-13-8	40
4			Acetonitrile, isothiocyanato-	98	C3H2N2S	032772-75-1	38
5			Benzen-d5-amine	98	C6H2D5N	004165-61-1	37

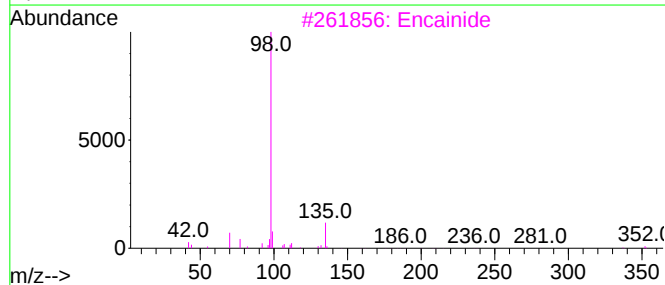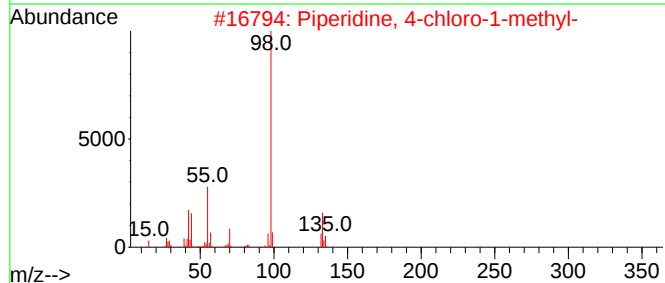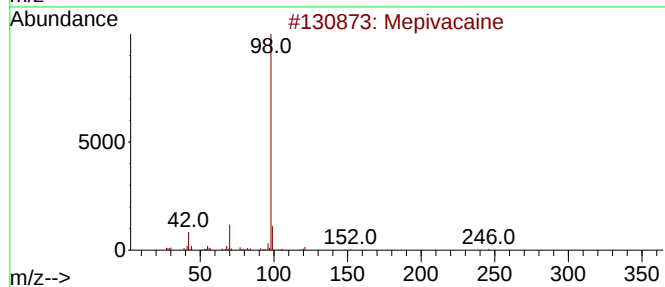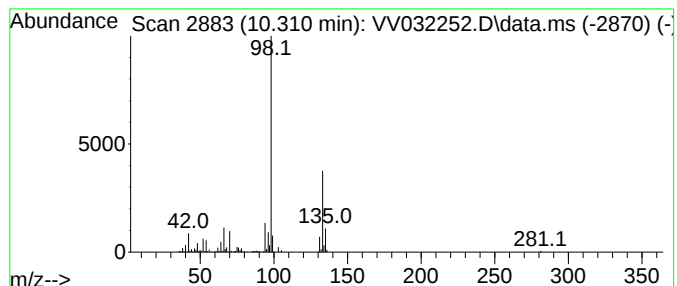

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032252.D
Acq On : 05 Oct 2023 13:43
Operator : SY/MD
Sample : 04744-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH580










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown-02 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.426	0.90 ug/L	98054	1,4-Dichlorobenzene-d4	11.188

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Encainide	352	C22H28N2O2	037612-13-8	47
2			Mepivacaine	246	C15H22N2O	000096-88-8	38
3			1,2-Cyclopentanedione	98	C5H6O2	003008-40-0	38
4			Acetonitrile, isothiocyanato-	98	C3H2N2S	032772-75-1	38
5			Mepivacaine	246	C15H22N2O	000096-88-8	38

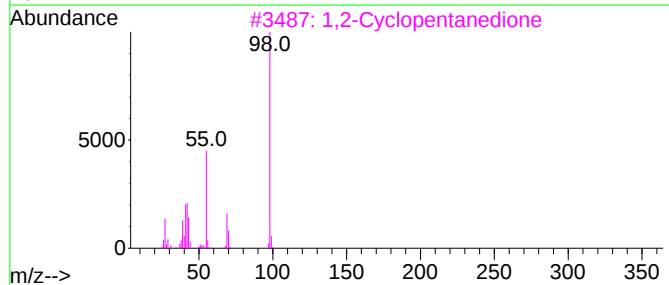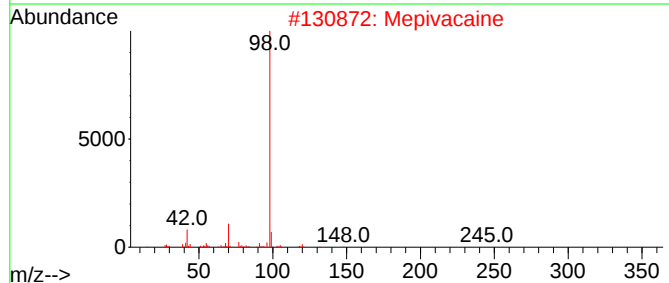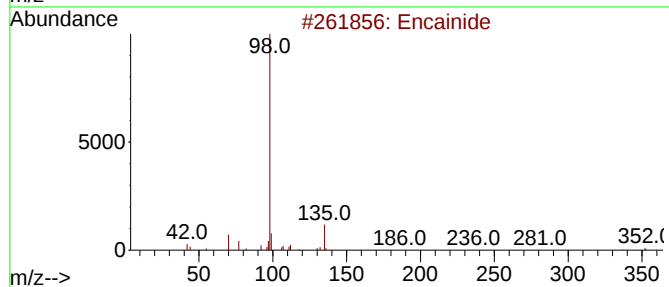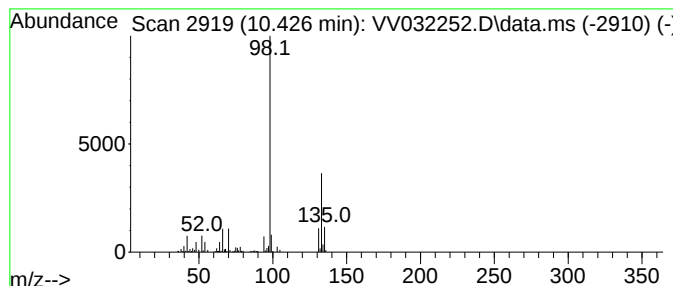

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032252.D
Acq On : 05 Oct 2023 13:43
Operator : SY/MD
Sample : 04744-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH580

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	10.310	2.2	ug/L	242683	3	11.188	543352	5.0
unknown-02	10.426	0.9	ug/L	98054	3	11.188	543352	5.0