

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
 Data File : VV032253.D
 Acq On : 05 Oct 2023 14:07
 Operator : SY/MD
 Sample : 04744-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH581

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032253.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rVB	47803	51420	13.85%	1.770%
2	1.532	144	153	168	rBV	43473	51547	13.88%	1.774%
3	2.060	307	317	332	rBV	76765	111537	30.03%	3.839%
4	3.815	850	863	897	rBV2	40477	155883	41.97%	5.365%
5	4.256	983	1000	1030	rBV	53799	145073	39.06%	4.993%
6	4.963	1203	1220	1250	rBV2	128083	336896	90.71%	11.596%
7	5.539	1388	1399	1422	rBV	105366	223105	60.07%	7.679%
8	5.831	1480	1490	1502	rBV5	4961	9674	2.60%	0.333%
9	5.992	1527	1540	1571	rBV	75977	168383	45.34%	5.796%
10	6.921	1819	1829	1857	rBV	33994	68434	18.43%	2.355%
11	7.249	1918	1931	1961	rBV	142942	269391	72.54%	9.272%
12	7.561	2019	2028	2054	rBV2	19513	39038	10.51%	1.344%
13	7.882	2121	2128	2138	rVB3	2413	4174	1.12%	0.144%
14	8.034	2165	2175	2216	rBV2	165869	371383	100.00%	12.783%
15	8.789	2399	2410	2435	rBV	171247	288667	77.73%	9.936%
16	10.159	2825	2836	2851	rBV	54038	87158	23.47%	3.000%
17	10.326	2880	2888	2899	rVB4	4655	7430	2.00%	0.256%
18	11.188	3146	3156	3178	rBV	174717	274823	74.00%	9.459%
19	11.564	3262	3273	3291	rBV	150742	241340	64.98%	8.307%




Sum of corrected areas: 2905356

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032253.D
Acq On : 05 Oct 2023 14:07
Operator : SY/MD
Sample : 04744-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH581

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

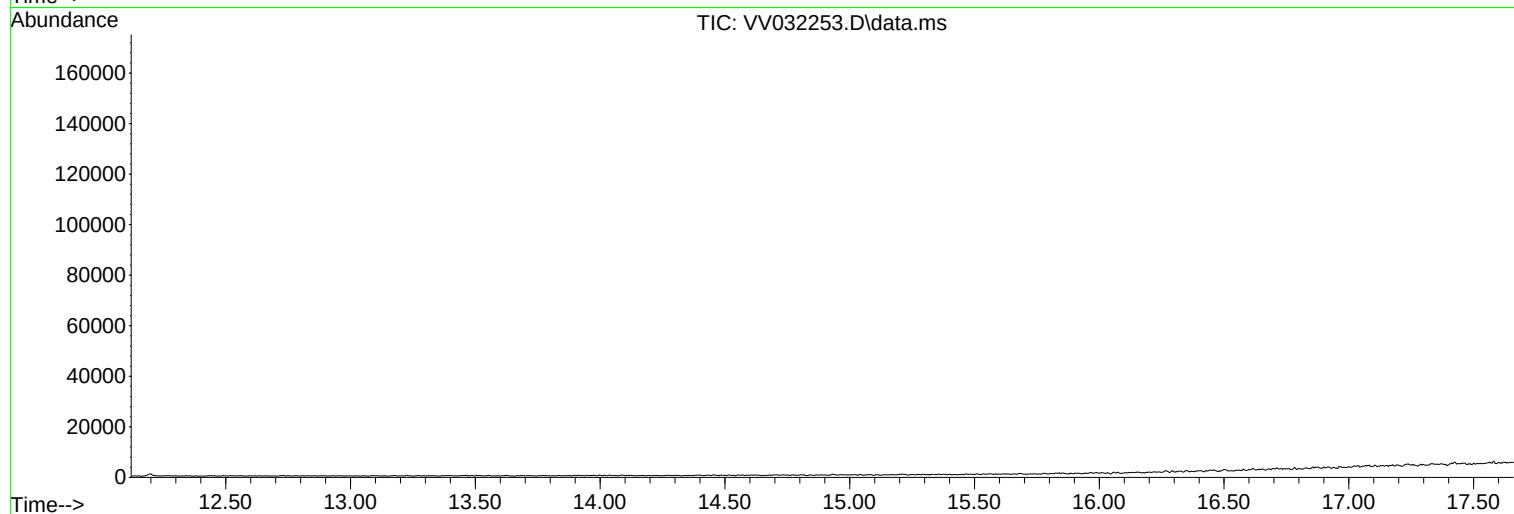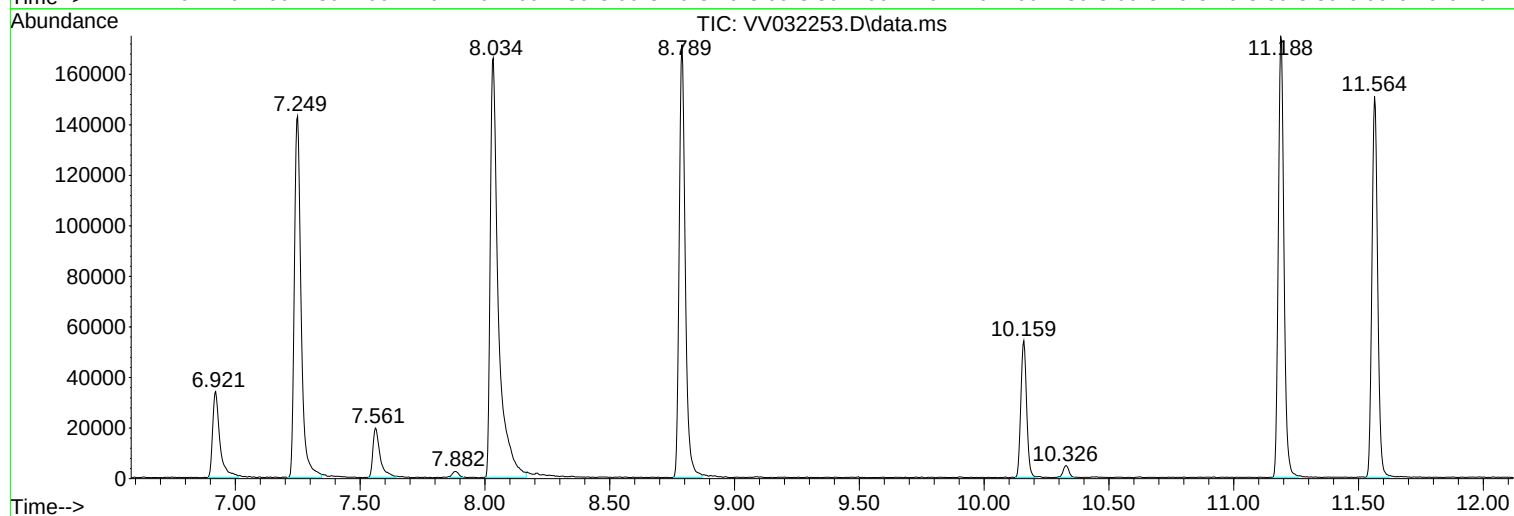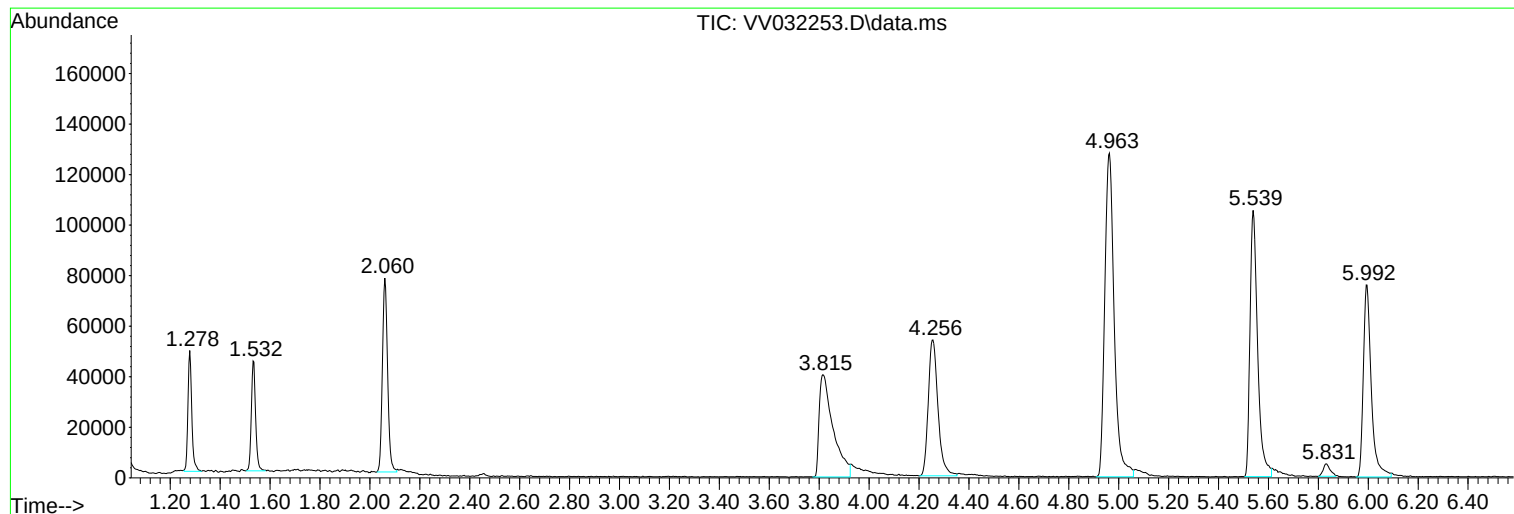

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032253.D
Acq On : 05 Oct 2023 14:07
Operator : SY/MD
Sample : 04744-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH581

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032253.D
Acq On : 05 Oct 2023 14:07
Operator : SY/MD
Sample : 04744-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH581

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc