

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
 Data File : VV032265.D
 Acq On : 05 Oct 2023 19:01
 Operator : SY/MD
 Sample : 04748-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX886

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032265.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rVB	45572	50073	4.31%	1.103%
2	1.532	146	153	167	rVB	43575	52076	4.48%	1.147%
3	2.059	307	317	329	rBV	69180	100881	8.68%	2.223%
4	3.802	849	859	892	rBV2	50845	162758	14.00%	3.586%
5	4.278	984	1007	1027	rBV3	138277	445132	38.29%	9.807%
6	4.516	1070	1081	1100	rVB5	5590	14068	1.21%	0.310%
7	4.738	1129	1150	1167	rBV	473551	1162638	100.00%	25.614%
8	4.825	1170	1177	1201	rVB2	31632	87317	7.51%	1.924%
9	4.963	1204	1220	1238	rBV2	122206	307434	26.44%	6.773%
10	5.538	1387	1399	1417	rBV	97910	207023	17.81%	4.561%
11	5.837	1479	1492	1507	rBV	93272	196627	16.91%	4.332%
12	5.992	1529	1540	1555	rBV	70249	146808	12.63%	3.234%
13	6.921	1819	1829	1847	rBV2	31936	63776	5.49%	1.405%
14	7.249	1920	1931	1950	rBV	140671	261755	22.51%	5.767%
15	7.561	2019	2028	2057	rBV	18544	38413	3.30%	0.846%
16	8.030	2164	2174	2209	rBV	183591	375668	32.31%	8.276%
17	8.789	2399	2410	2435	rBV	159602	277891	23.90%	6.122%
18	10.159	2824	2836	2855	rBV	58535	94252	8.11%	2.076%
19	11.191	3146	3157	3180	rBV	164769	260714	22.42%	5.744%
20	11.564	3263	3273	3295	rBV	147008	233746	20.10%	5.150%




Sum of corrected areas: 4539050

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032265.D
Acq On : 05 Oct 2023 19:01
Operator : SY/MD
Sample : 04748-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX886

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

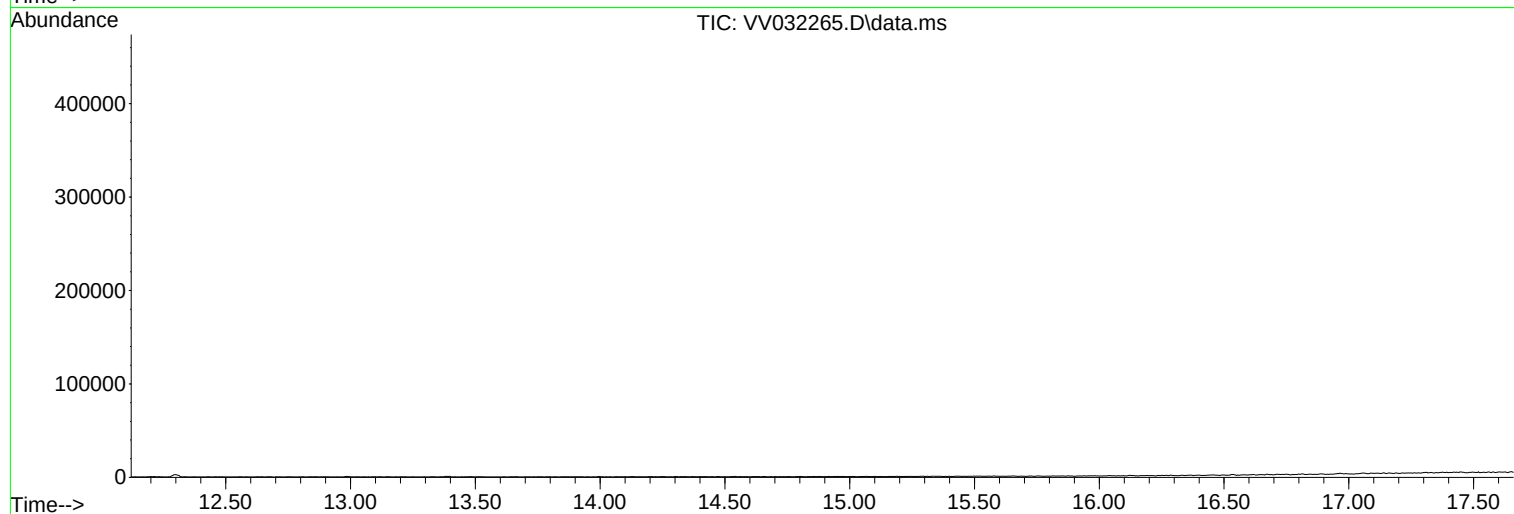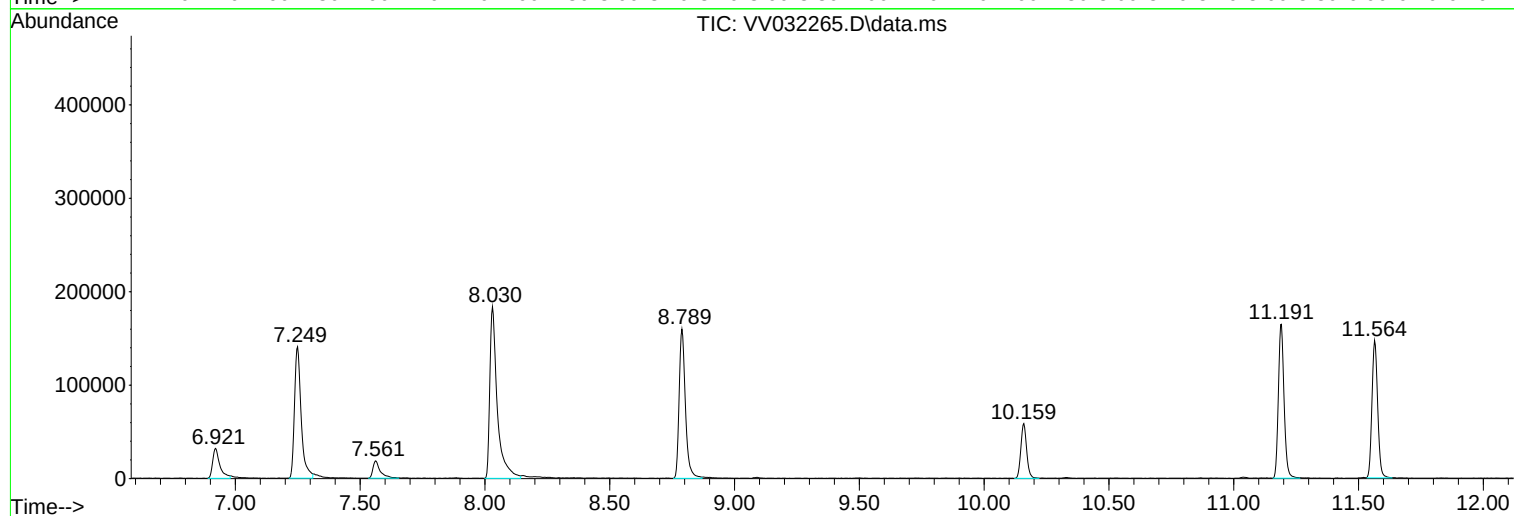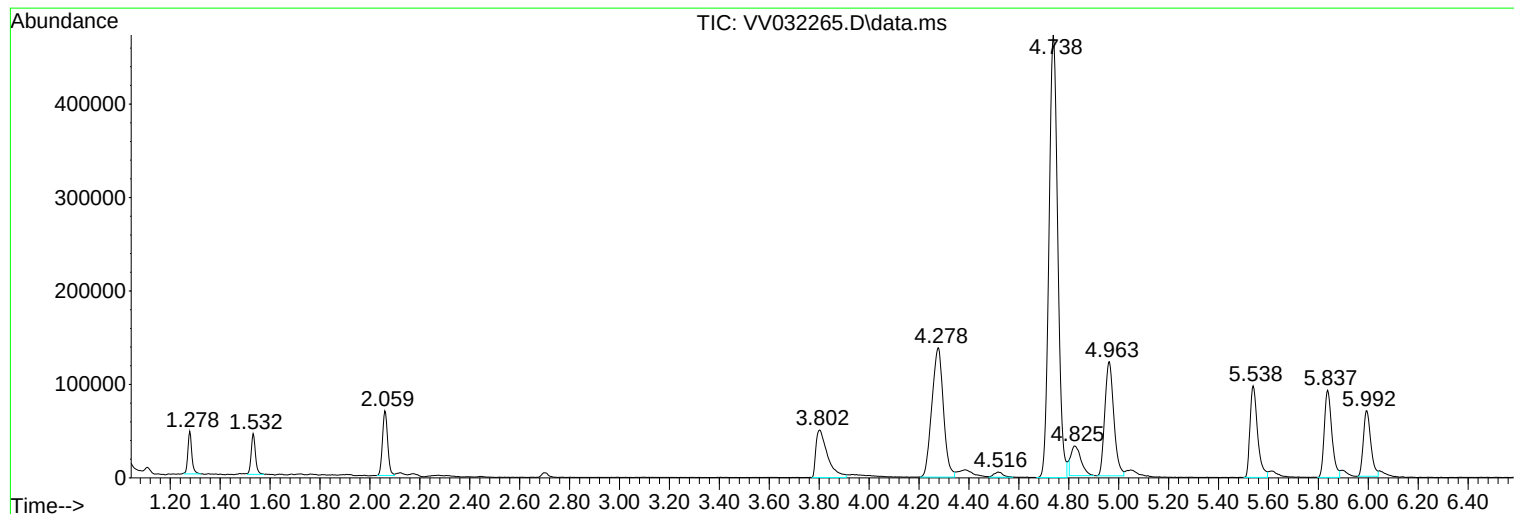

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032265.D
Acq On : 05 Oct 2023 19:01
Operator : SY/MD
Sample : 04748-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX886

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032265.D
Acq On : 05 Oct 2023 19:01
Operator : SY/MD
Sample : 04748-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX886

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc