

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
 Data File : VV032272.D
 Acq On : 05 Oct 2023 22:12
 Operator : SY/MD
 Sample : 04741-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032272.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	86	rVB	39969	42548	12.25%	1.611%
2	1.532	146	153	167	rVB	38925	47096	13.56%	1.783%
3	2.056	307	316	329	rBV	65149	94675	27.26%	3.584%
4	3.828	856	867	903	rBV	26603	124177	35.76%	4.701%
5	4.252	983	999	1024	rBV3	48653	128724	37.07%	4.874%
6	4.355	1024	1031	1047	rVB7	1792	4517	1.30%	0.171%
7	4.960	1204	1219	1240	rBV3	114320	293063	84.40%	11.095%
8	5.539	1388	1399	1417	rBV	96351	201936	58.15%	7.645%
9	5.838	1480	1492	1507	rVB7	4278	9609	2.77%	0.364%
10	5.992	1527	1540	1556	rBV	65224	142479	41.03%	5.394%
11	6.445	1671	1681	1695	rBV4	1990	3667	1.06%	0.139%
12	6.921	1819	1829	1856	rBV2	27764	59431	17.11%	2.250%
13	7.249	1920	1931	1966	rBV	125554	245287	70.64%	9.287%
14	7.561	2020	2028	2057	rBV	16040	33557	9.66%	1.270%
15	7.911	2127	2137	2158	rVB3	17650	33862	9.75%	1.282%
16	8.034	2165	2175	2213	rBV	153108	347246	100.00%	13.147%
17	8.185	2213	2222	2230	rVB2	3787	7484	2.16%	0.283%
18	8.789	2398	2410	2440	rBV	156462	271782	78.27%	10.290%
19	10.159	2825	2836	2855	rVB	52795	85881	24.73%	3.251%
20	11.188	3146	3156	3178	rBV	156310	250611	72.17%	9.488%
21	11.564	3259	3273	3294	rBV	135372	213672	61.53%	8.090%




Sum of corrected areas: 2641304

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032272.D
Acq On : 05 Oct 2023 22:12
Operator : SY/MD
Sample : 04741-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

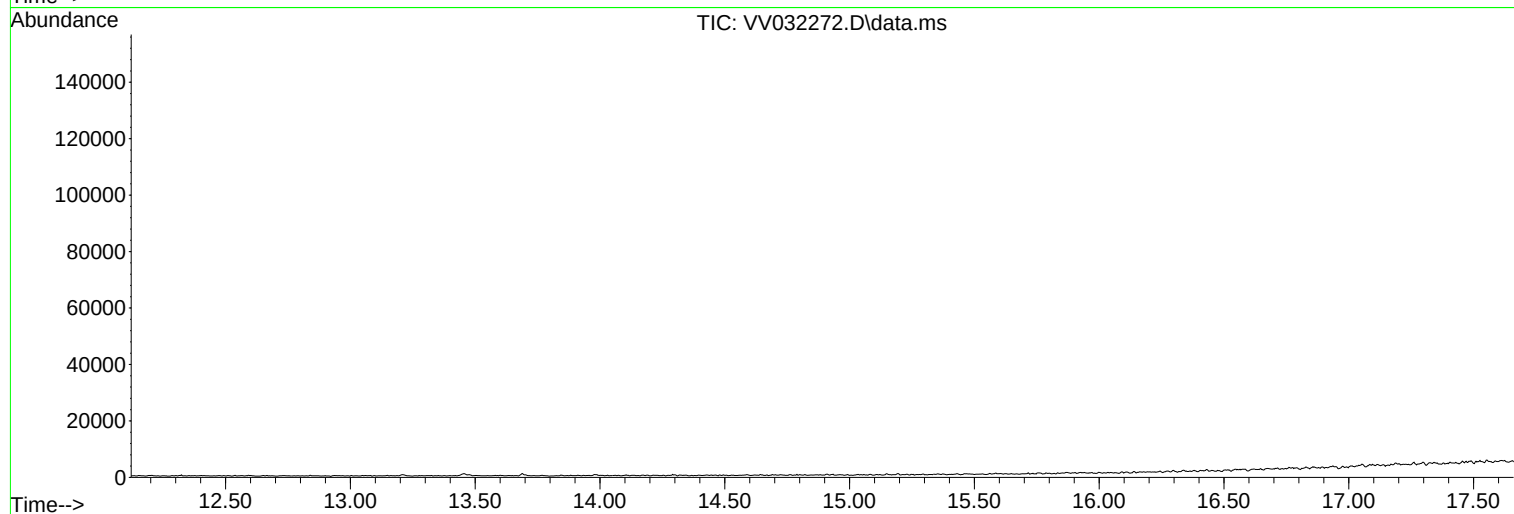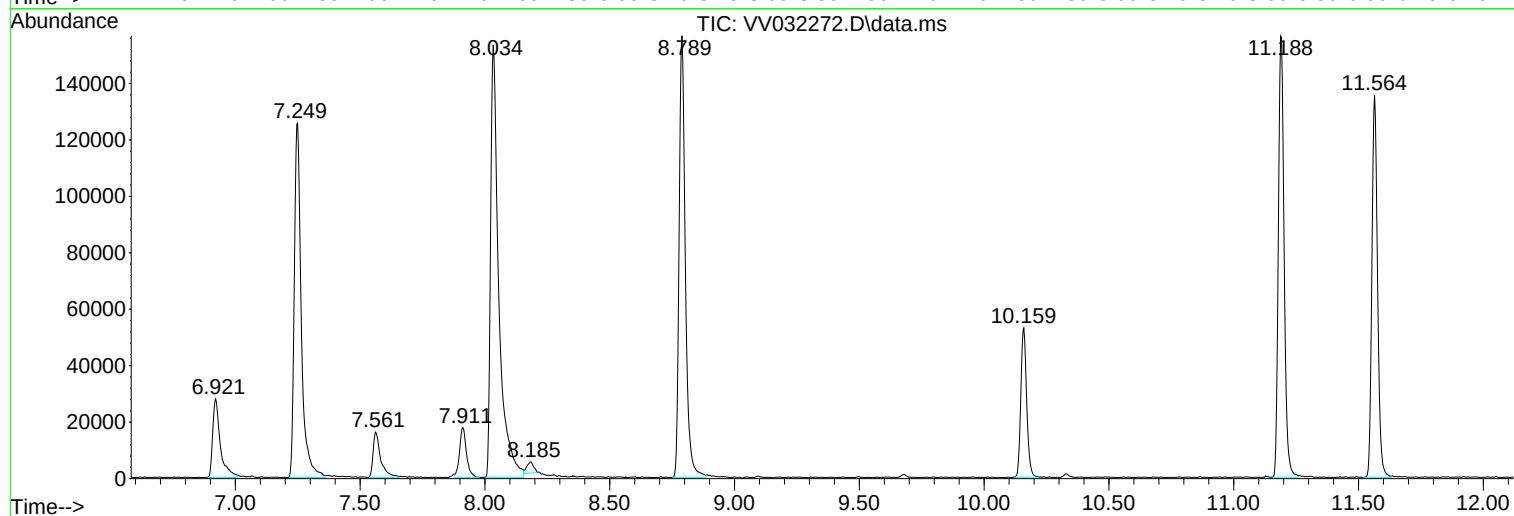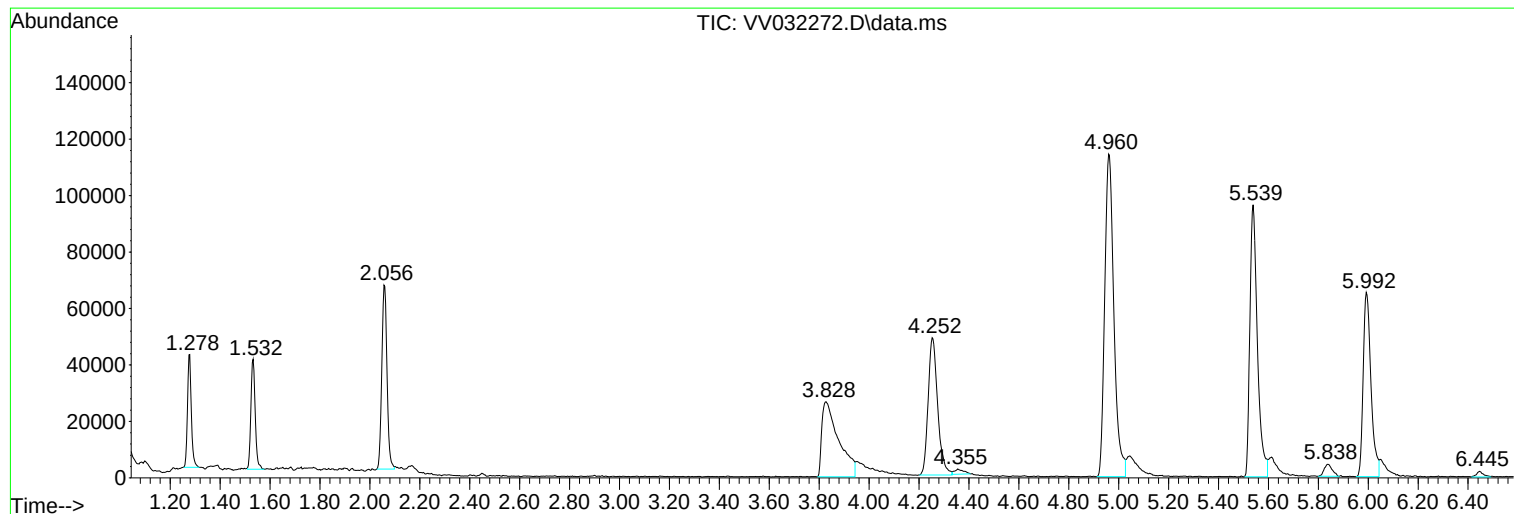

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032272.D
Acq On : 05 Oct 2023 22:12
Operator : SY/MD
Sample : 04741-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032272.D
Acq On : 05 Oct 2023 22:12
Operator : SY/MD
Sample : 04741-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------