

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
 Data File : VV032273.D
 Acq On : 05 Oct 2023 22:36
 Operator : SY/MD
 Sample : 04741-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032273.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	66	74	86	rBV	42775	46340	13.06%	1.670%
2	1.532	145	153	167	rBV	40962	47040	13.26%	1.695%
3	2.059	307	317	332	rBV	67682	98034	27.64%	3.532%
4	3.825	855	866	913	rBV	29869	139775	39.41%	5.036%
5	4.252	984	999	1022	rBV	50427	137177	38.67%	4.943%
6	4.355	1027	1031	1047	rVB4	1911	4188	1.18%	0.151%
7	4.960	1204	1219	1240	rBV2	119107	304440	85.83%	10.969%
8	5.538	1387	1399	1419	rBV	98529	211018	59.49%	7.603%
9	5.837	1480	1492	1505	rBV	3995	9381	2.64%	0.338%
10	5.992	1525	1540	1556	rBV	67146	147074	41.47%	5.299%
11	6.442	1670	1680	1701	rBV3	6825	14466	4.08%	0.521%
12	6.921	1818	1829	1856	rBV2	28044	60927	17.18%	2.195%
13	7.249	1920	1931	1960	rBV	131153	254599	71.78%	9.173%
14	7.561	2018	2028	2048	rBV3	16450	34622	9.76%	1.247%
15	7.911	2121	2137	2150	rBV3	16303	32959	9.29%	1.188%
16	8.034	2166	2175	2212	rBV	157939	354692	100.00%	12.780%
17	8.181	2213	2221	2236	rVB2	10256	20796	5.86%	0.749%
18	8.789	2400	2410	2435	rBV	161088	279813	78.89%	10.082%
19	9.677	2677	2686	2696	rVB4	2302	3629	1.02%	0.131%
20	10.159	2825	2836	2853	rBV	54282	87784	24.75%	3.163%
21	10.329	2877	2889	2899	rBV4	4751	7475	2.11%	0.269%
22	11.188	3146	3156	3175	rBV	158460	256668	72.36%	9.248%
23	11.564	3260	3273	3291	rBV	140155	222499	62.73%	8.017%




Sum of corrected areas: 2775396

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032273.D
Acq On : 05 Oct 2023 22:36
Operator : SY/MD
Sample : 04741-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

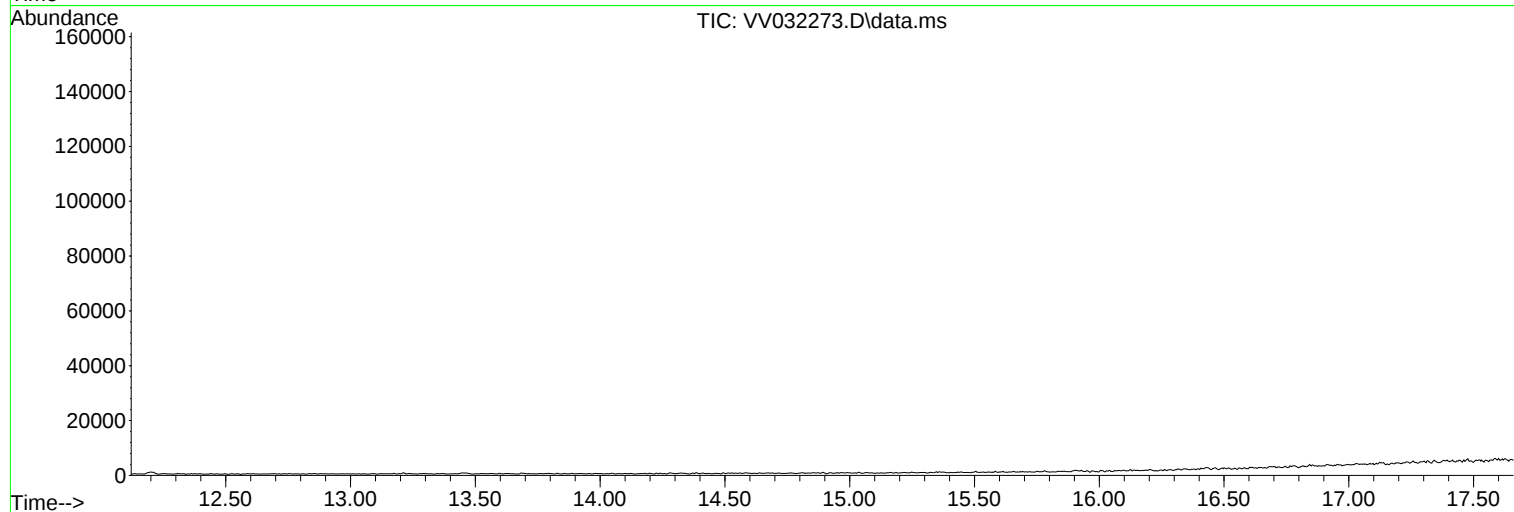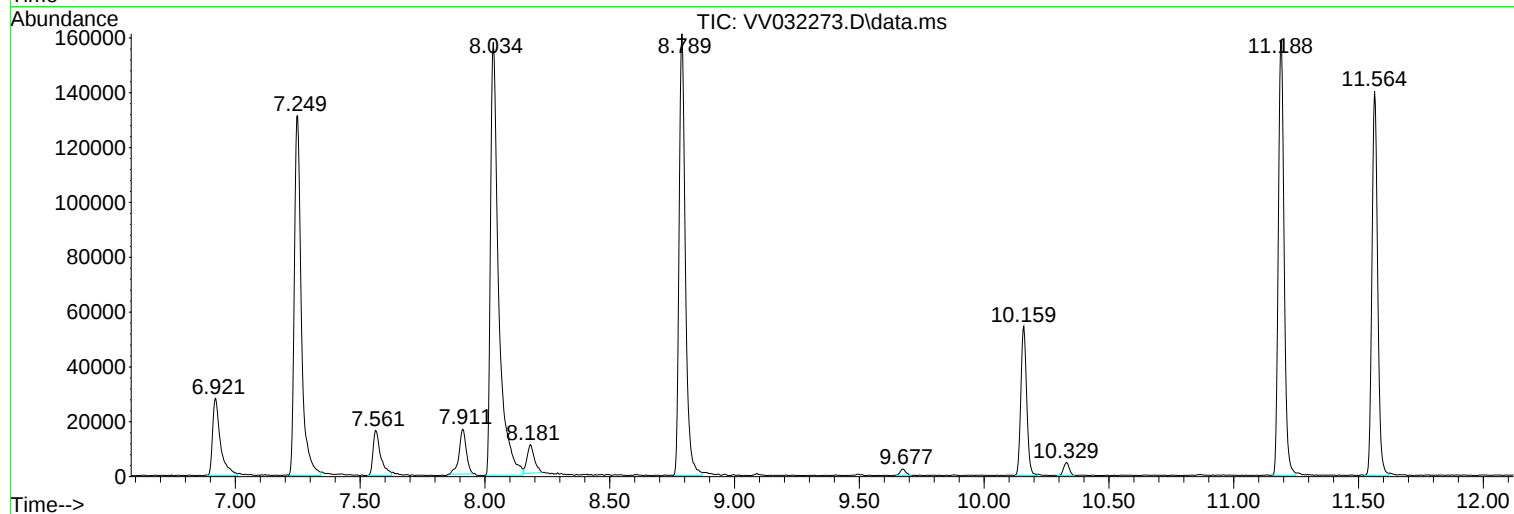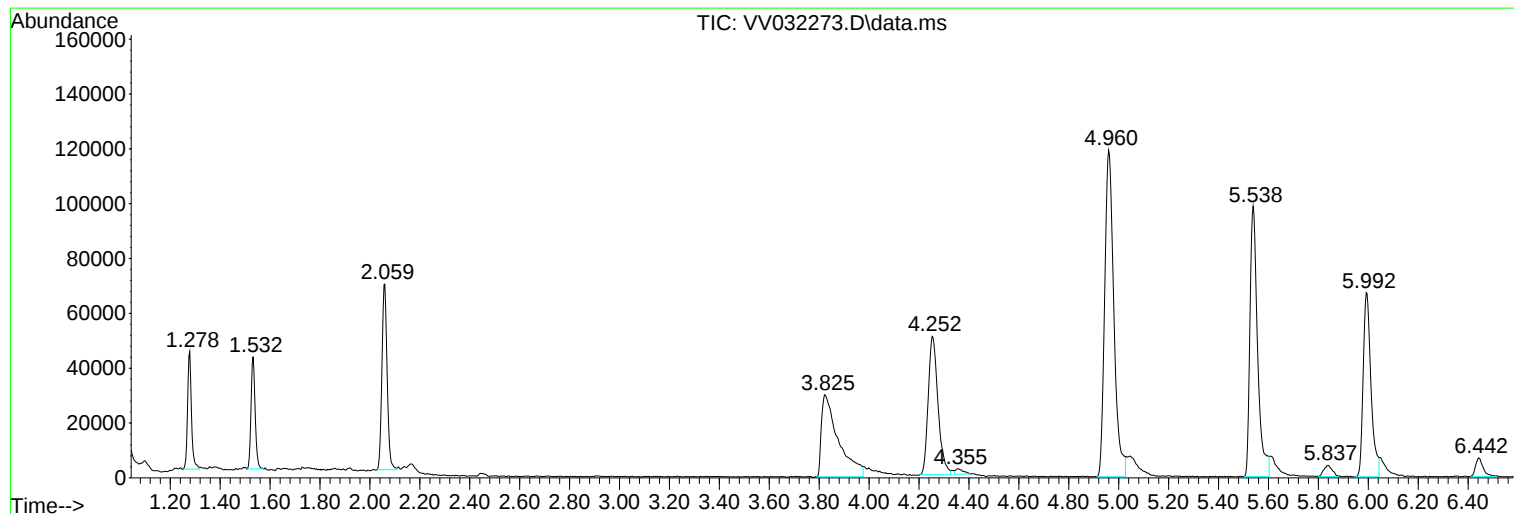

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032273.D
Acq On : 05 Oct 2023 22:36
Operator : SY/MD
Sample : 04741-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032273.D
Acq On : 05 Oct 2023 22:36
Operator : SY/MD
Sample : 04741-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc