

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
 Data File : VV032275.D
 Acq On : 05 Oct 2023 23:25
 Operator : SY/MD
 Sample : 04741-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032275.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	66	74	87	rBV	41880	45654	13.12%	1.578%
2	1.532	145	153	163	rBV	40814	47316	13.60%	1.636%
3	2.060	307	317	330	rBV	67038	97218	27.94%	3.361%
4	3.818	853	864	905	rBV	31347	134900	38.76%	4.663%
5	4.256	982	1000	1025	rBV4	54988	171016	49.14%	5.912%
6	4.960	1203	1219	1238	rBV3	114622	292854	84.15%	10.124%
7	5.539	1387	1399	1415	rBV	97276	203664	58.52%	7.041%
8	5.834	1482	1491	1504	rBV7	3814	7971	2.29%	0.276%
9	5.992	1528	1540	1569	rBV	67272	156357	44.93%	5.405%
10	6.439	1664	1679	1700	rBV2	28425	60338	17.34%	2.086%
11	6.921	1819	1829	1860	rBV	28279	60246	17.31%	2.083%
12	7.246	1918	1930	1952	rBV	130194	247069	71.00%	8.541%
13	7.561	2020	2028	2051	rBV2	16734	33682	9.68%	1.164%
14	7.908	2122	2136	2157	rVB2	45345	84135	24.18%	2.908%
15	8.034	2164	2175	2209	rBV	155678	348005	100.00%	12.030%
16	8.182	2212	2221	2235	rVB2	27242	50170	14.42%	1.734%
17	8.789	2399	2410	2436	rBV	158925	278146	79.93%	9.615%
18	9.670	2675	2684	2698	rBV4	5550	9811	2.82%	0.339%
19	10.156	2825	2835	2852	rBV2	54615	87023	25.01%	3.008%
20	11.188	3145	3156	3175	rBV	160782	257422	73.97%	8.899%
21	11.564	3261	3273	3293	rBV	139511	219746	63.14%	7.596%




Sum of corrected areas: 2892743

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032275.D
Acq On : 05 Oct 2023 23:25
Operator : SY/MD
Sample : 04741-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

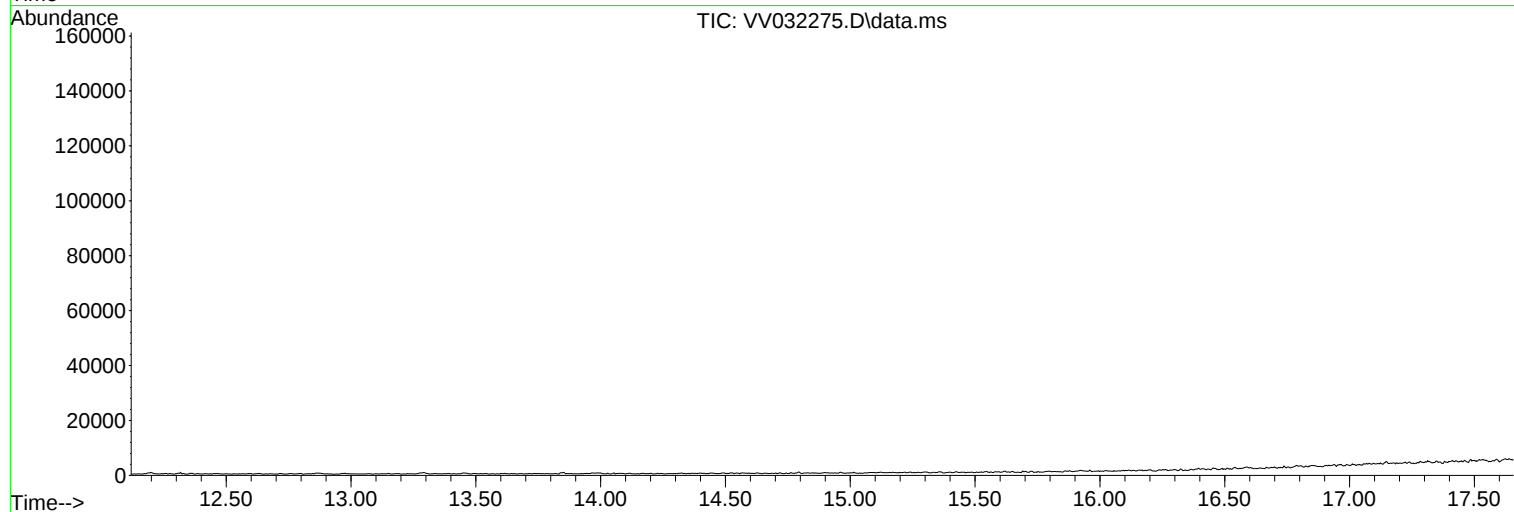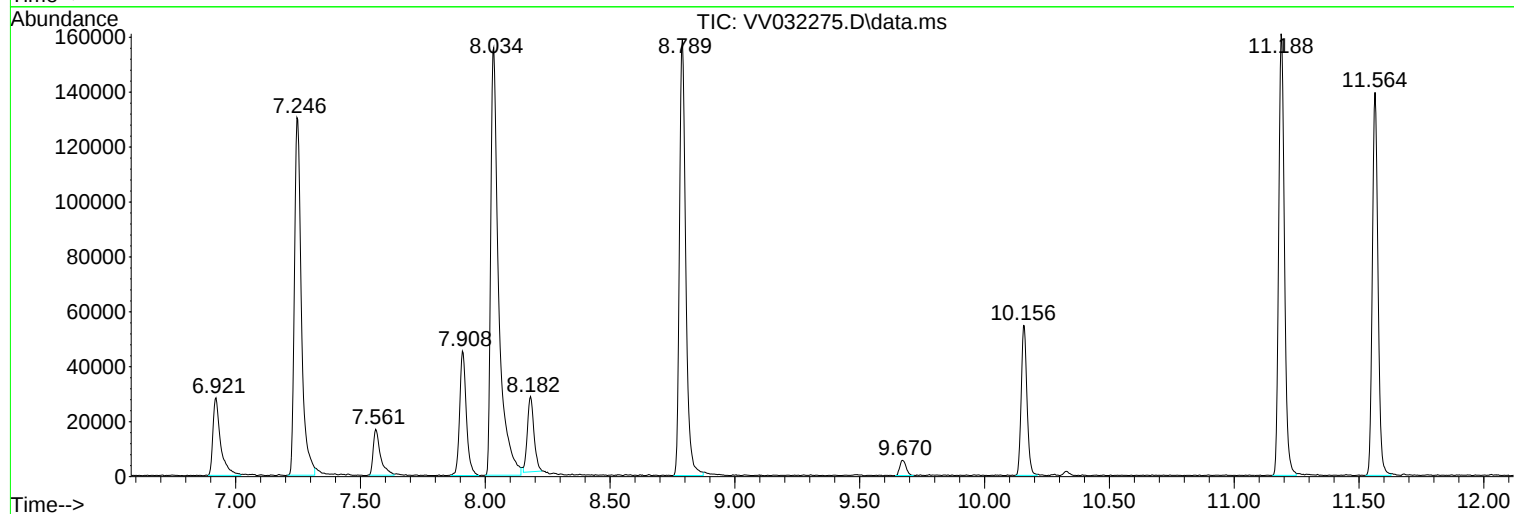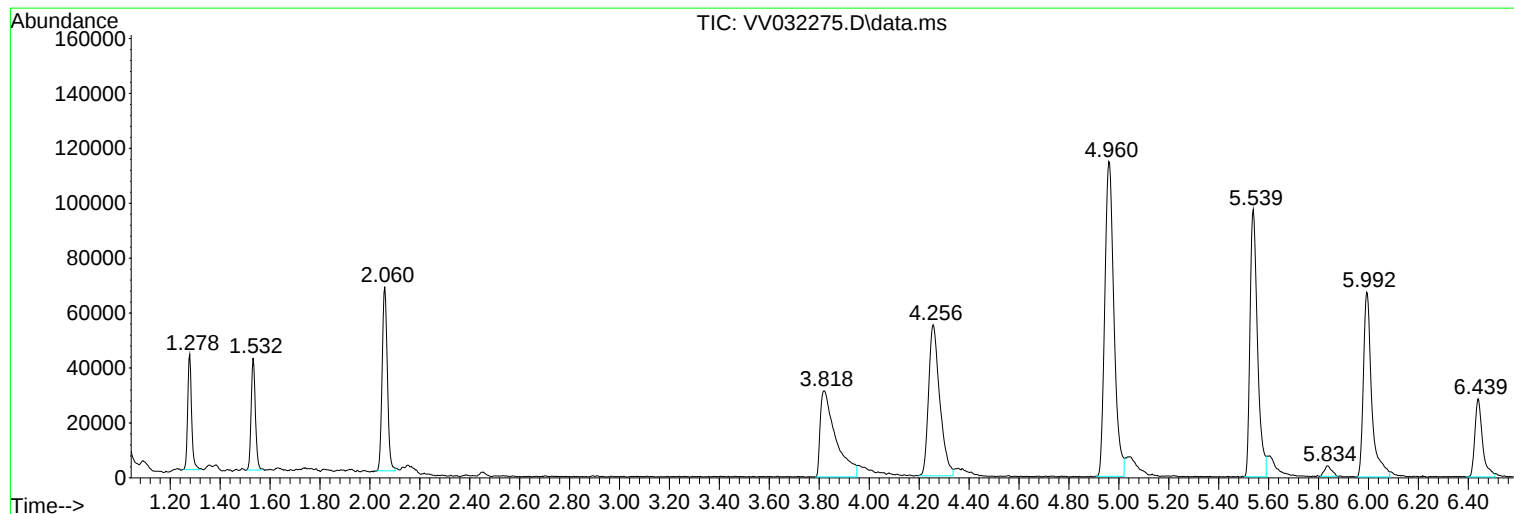

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032275.D
Acq On : 05 Oct 2023 23:25
Operator : SY/MD
Sample : 04741-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032275.D
Acq On : 05 Oct 2023 23:25
Operator : SY/MD
Sample : 04741-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc