

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
 Data File : VV032276.D
 Acq On : 05 Oct 2023 23:50
 Operator : SY/MD
 Sample : 04741-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032276.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	86	rBV	41788	45891	12.90%	1.683%
2	1.532	146	153	167	rVB	40136	47800	13.44%	1.753%
3	2.057	307	316	333	rBV	67466	99113	27.87%	3.636%
4	3.825	853	866	916	rBV2	29662	142254	40.00%	5.218%
5	4.253	983	999	1023	rBV	49800	133505	37.54%	4.897%
6	4.960	1203	1219	1238	rBV2	115276	296826	83.46%	10.889%
7	5.539	1387	1399	1417	rBV	96027	204356	57.46%	7.497%
8	5.834	1481	1491	1506	rBV7	3907	8368	2.35%	0.307%
9	5.992	1527	1540	1568	rBV2	67536	156289	43.94%	5.733%
10	6.918	1818	1828	1850	rBV2	28357	59592	16.76%	2.186%
11	7.246	1920	1930	1961	rBV	129709	250315	70.38%	9.182%
12	7.561	2020	2028	2051	rBV	16409	33781	9.50%	1.239%
13	7.912	2118	2137	2155	rVB4	19074	38428	10.80%	1.410%
14	8.034	2163	2175	2211	rBV	160322	355657	100.00%	13.047%
15	8.182	2214	2221	2236	rVB3	6222	12573	3.54%	0.461%
16	8.789	2399	2410	2435	rBV	158530	273040	76.77%	10.016%
17	10.156	2825	2835	2850	rBV	53282	87312	24.55%	3.203%
18	10.329	2881	2889	2899	rVB3	2674	4086	1.15%	0.150%
19	11.188	3145	3156	3180	rBV	163761	255234	71.76%	9.363%
20	11.564	3261	3273	3293	rBV	139392	221587	62.30%	8.129%




Sum of corrected areas: 2726007

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032276.D
Acq On : 05 Oct 2023 23:50
Operator : SY/MD
Sample : 04741-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

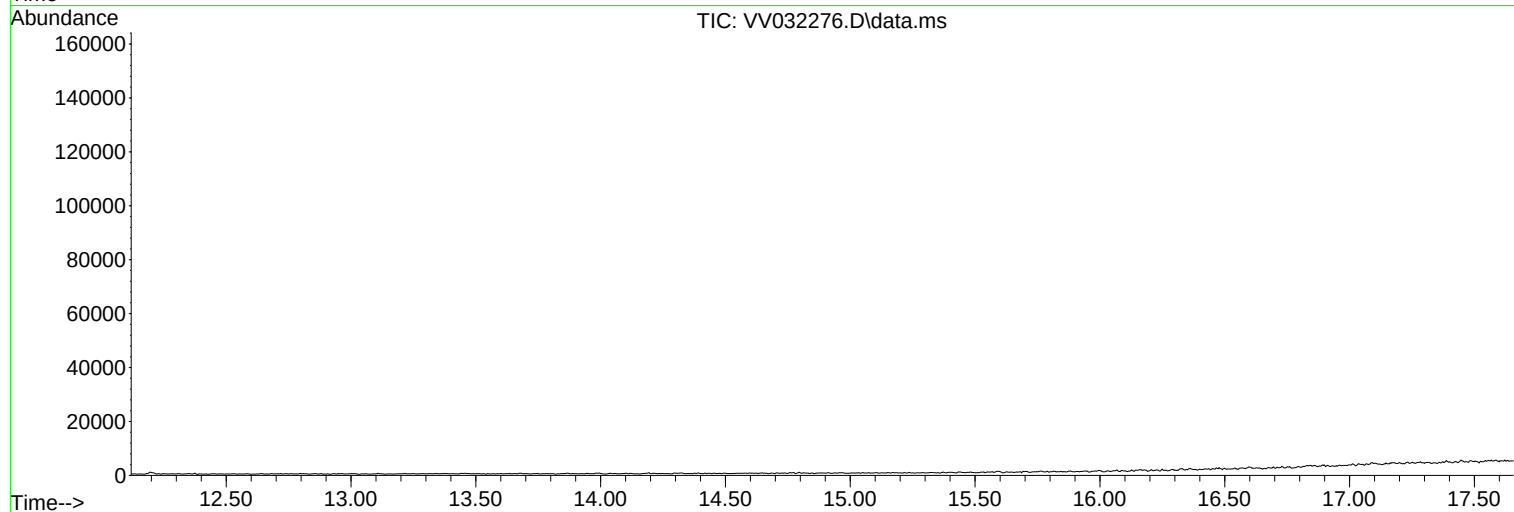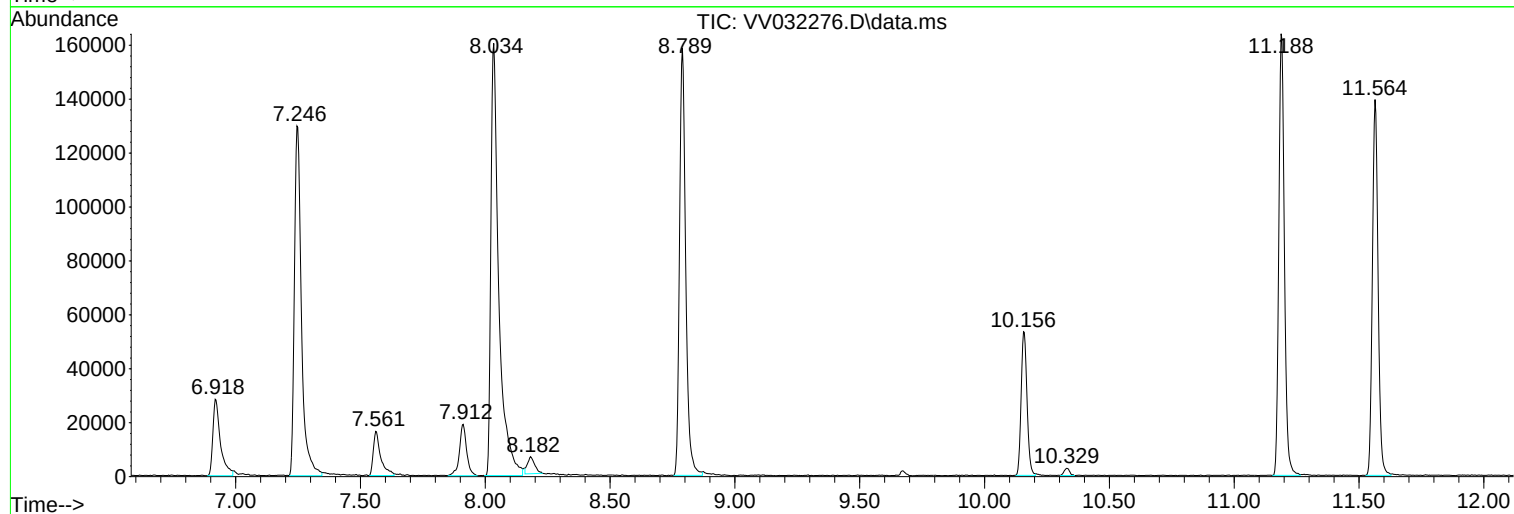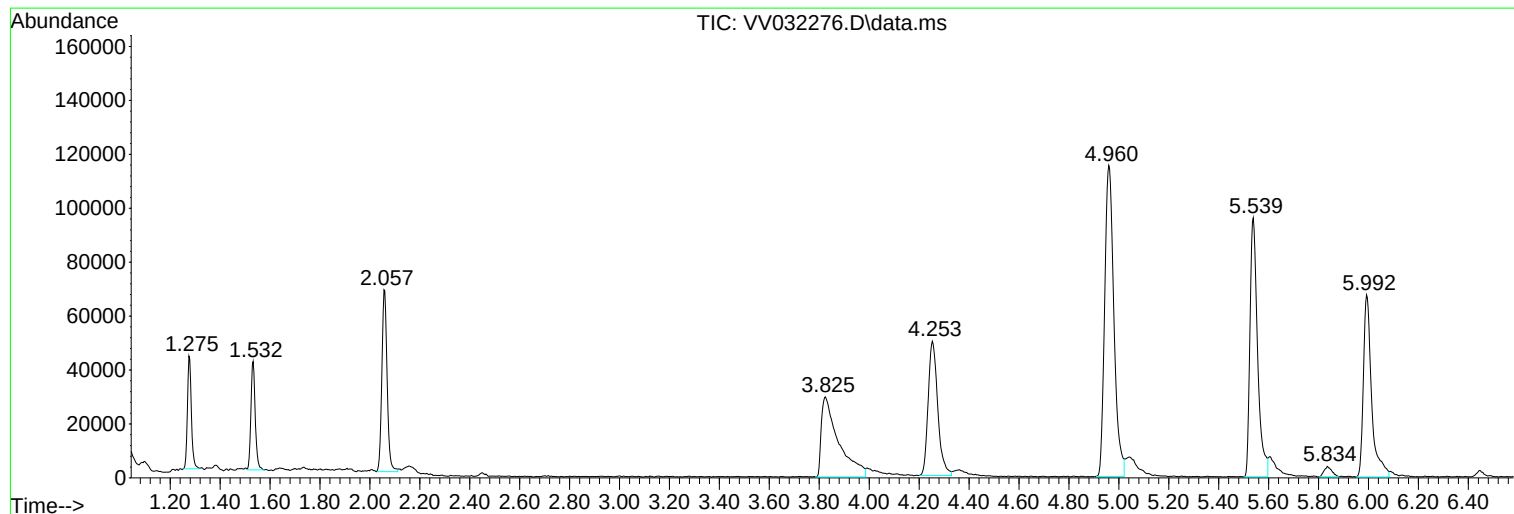

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032276.D
Acq On : 05 Oct 2023 23:50
Operator : SY/MD
Sample : 04741-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032276.D
Acq On : 05 Oct 2023 23:50
Operator : SY/MD
Sample : 04741-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------