

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
 Data File : VV032281.D
 Acq On : 06 Oct 2023 01:52
 Operator : SY/MD
 Sample : 04748-27
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX865

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032281.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	8	14	29	rVB	160865	177063	1.86%	1.392%
2	1.278	64	74	85	rBV	123956	139704	1.47%	1.098%
3	2.060	307	317	332	rBV2	67417	105287	1.11%	0.828%
4	2.693	503	514	532	rBV	101564	176181	1.85%	1.385%
5	3.815	846	863	888	rBV3	102496	306535	3.23%	2.409%
6	4.253	980	999	1022	rBV2	54562	146311	1.54%	1.150%
7	4.960	1201	1219	1252	rBV2	131271	358136	3.77%	2.815%
8	5.539	1385	1399	1415	rBV	107969	221681	2.33%	1.742%
9	5.834	1473	1491	1504	rBV	4903006	9504716	100.00%	74.705%
10	5.995	1531	1541	1554	rVB	67595	127345	1.34%	1.001%
11	7.246	1918	1930	1945	rBV	137358	246591	2.59%	1.938%
12	8.037	2166	2176	2204	rBV	220077	428706	4.51%	3.370%
13	8.789	2399	2410	2429	rBV	152166	256834	2.70%	2.019%
14	10.159	2825	2836	2849	rBV	60819	95404	1.00%	0.750%
15	11.191	3146	3157	3174	rBV	148902	232045	2.44%	1.824%
16	11.564	3262	3273	3298	rVB	126739	200544	2.11%	1.576%




Sum of corrected areas: 12723083

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032281.D
Acq On : 06 Oct 2023 01:52
Operator : SY/MD
Sample : 04748-27
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX865

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

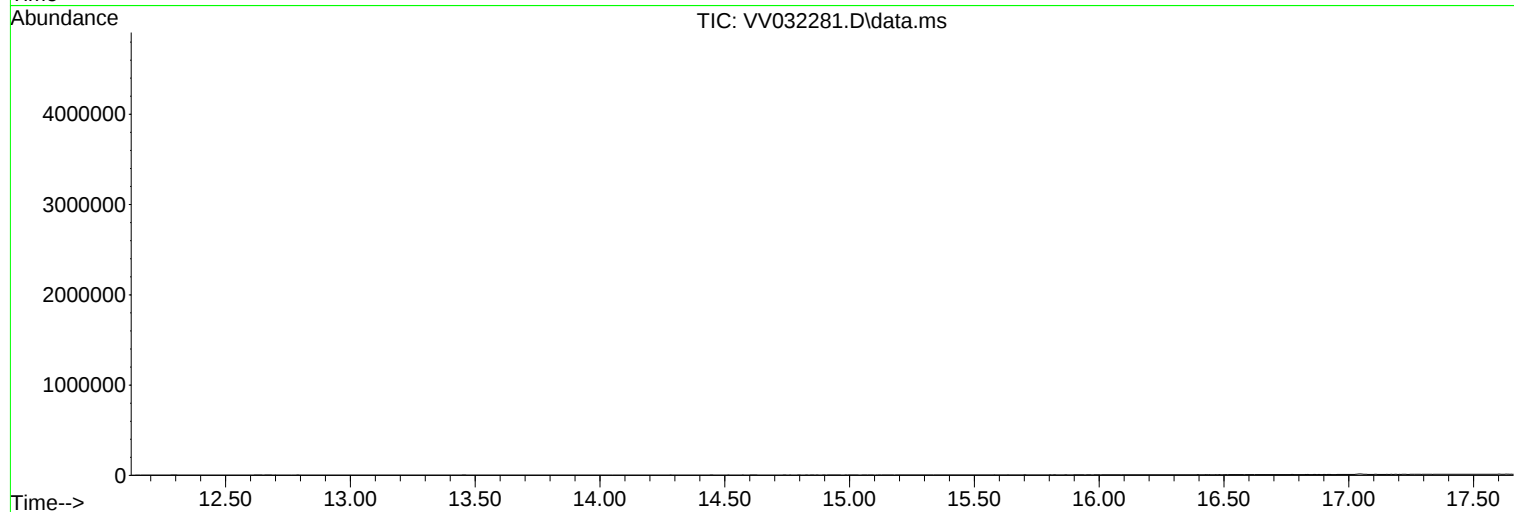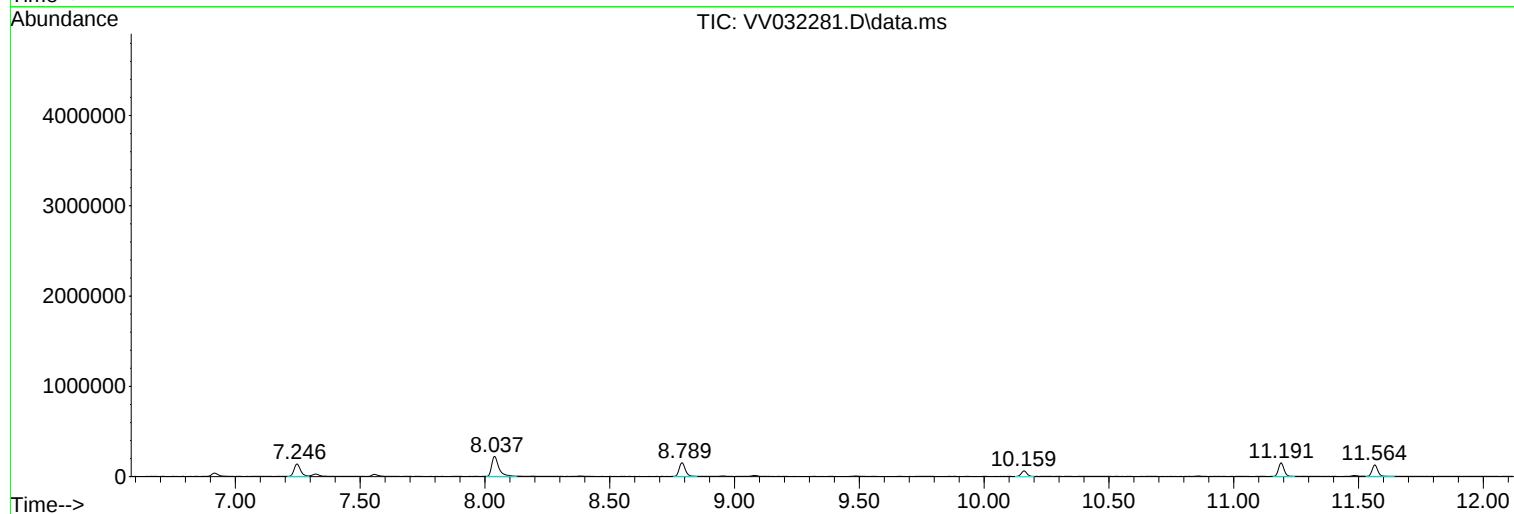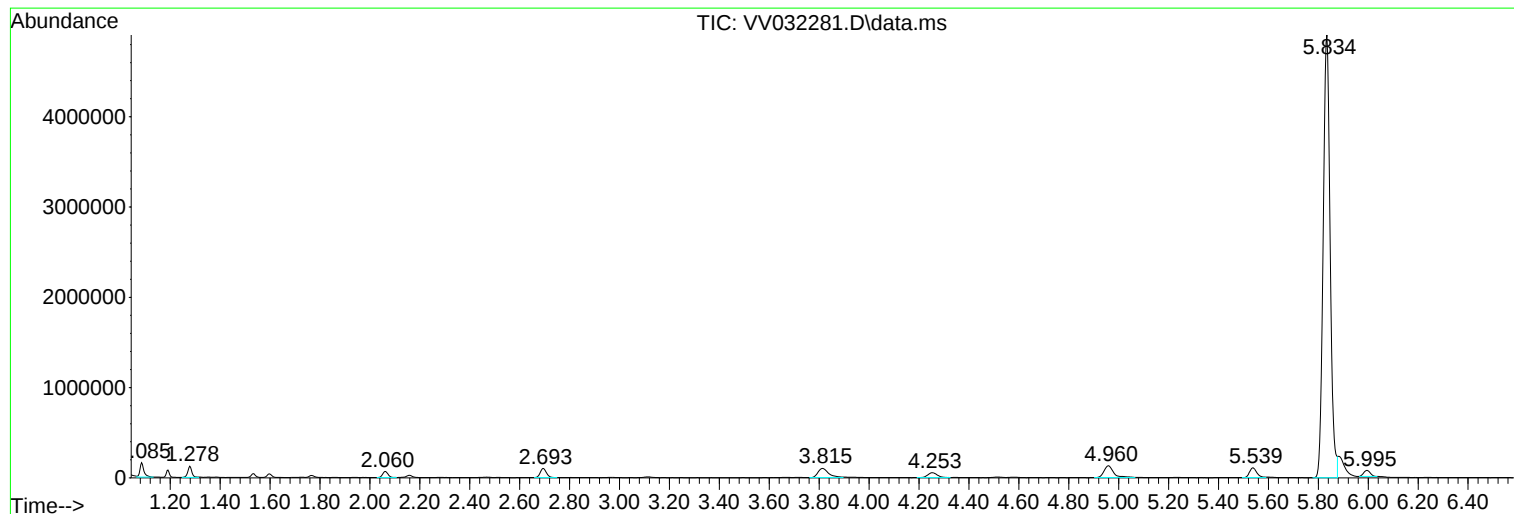

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032281.D
Acq On : 06 Oct 2023 01:52
Operator : SY/MD
Sample : 04748-27
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX865










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.085	3.99 ug/L	177063	1,4-Difluorobenzene	5.539

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane	44	C3H8	000074-98-6	74
2			Acetonitrile-d3	44	C2D3N	002206-26-0	9
3			Propene	42	C3H6	000115-07-1	9
4			Propane	44	C3H8	000074-98-6	7
5			Acetonitrile-d3	44	C2D3N	002206-26-0	4

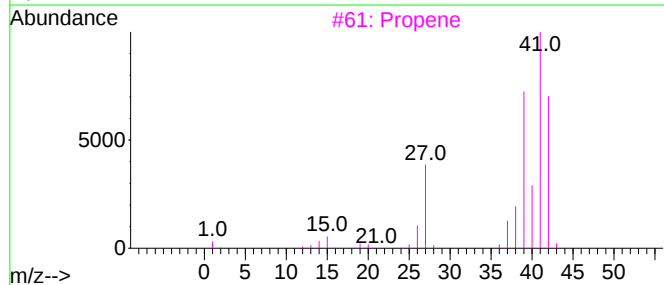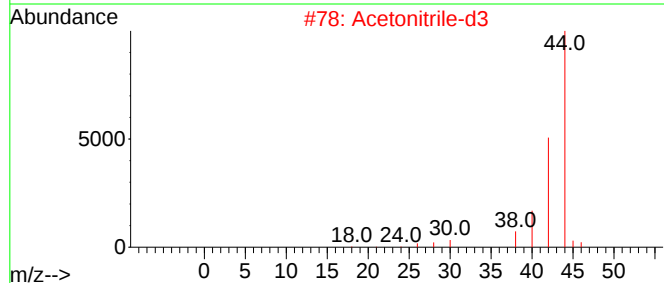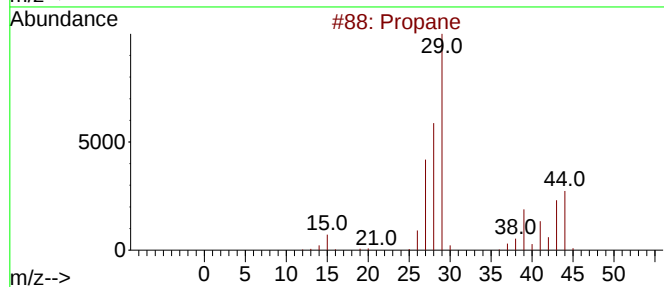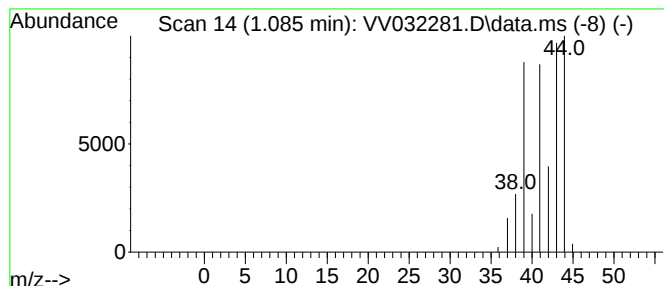

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032281.D
Acq On : 06 Oct 2023 01:52
Operator : SY/MD
Sample : 04748-27
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX865

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	1.085	4.0	ug/L	177063	1	5.539	221681	5.0