
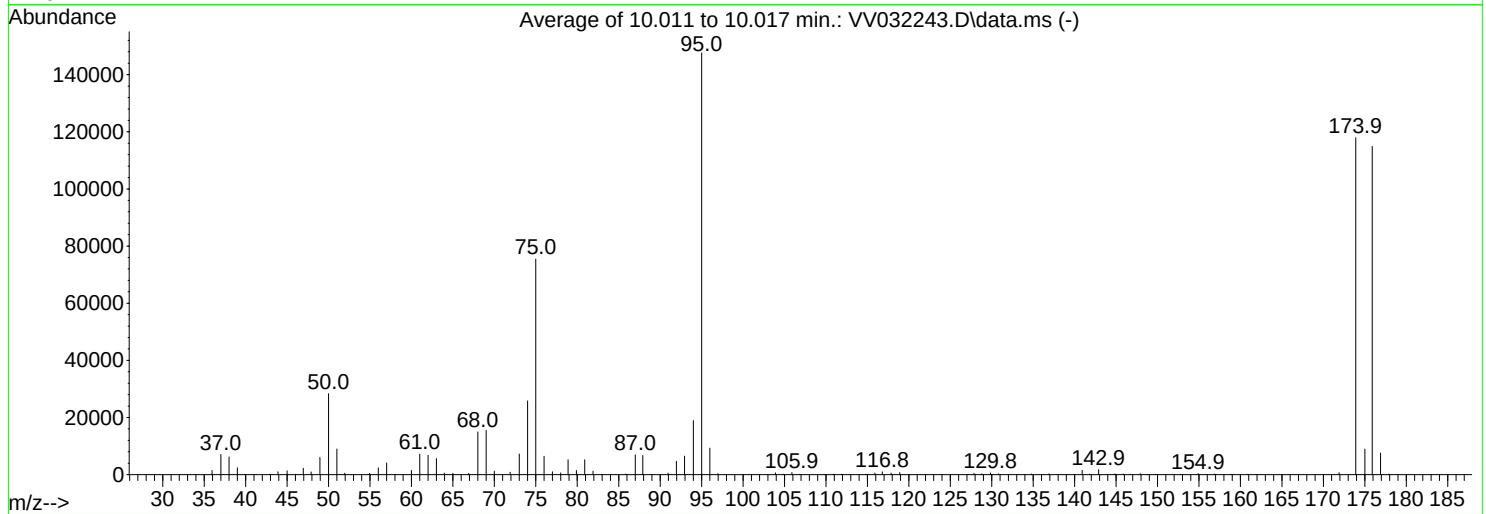


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032243.D
Acq On : 05 Oct 2023 09:21
Operator : SY/MD
Sample : BFB215
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB215

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Oct 06 05:25:10 2023

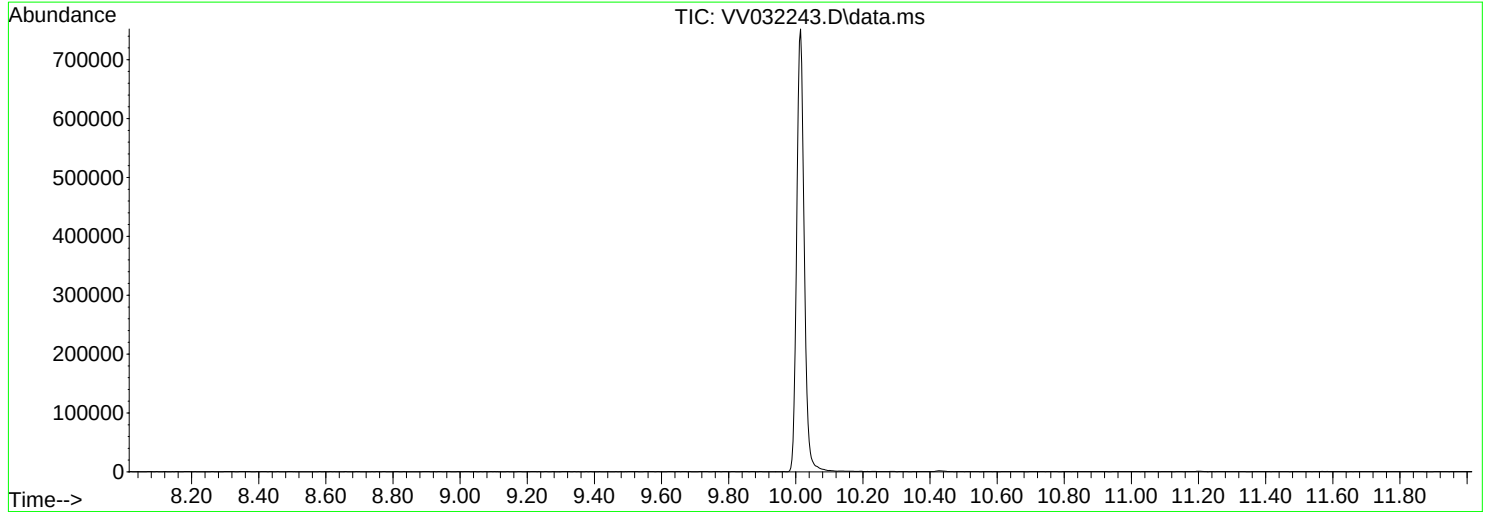

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	28360	PASS
75	95	30	80	51.1	75429	PASS
95	95	100	100	100.0	147648	PASS
96	95	5	9	6.3	9309	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.9	117933	PASS
175	174	5	9	7.6	8965	PASS
176	174	95	105	97.4	114859	PASS
177	176	5	10	6.6	7551	PASS

m/z	Abundance
39.90	124.0
43.90	289.0

Instrument :
MSVOA_V
ClientSampleId :
BFB215

m/z	Abundance
36.00	1477.0
37.00	7323.0
38.00	6593.0
39.00	2540.0
39.90	203.0
42.80	128.0
44.00	1273.0
45.00	1298.0
46.00	188.0
46.90	2259.0
47.90	881.0
49.00	6160.0
50.00	29384.0
51.00	9230.0
51.90	548.0
52.80	112.0
55.00	482.0
56.00	2507.0
57.00	4143.0
58.00	199.0
60.00	1447.0
61.00	7242.0
62.00	6974.0
63.00	5774.0
63.90	671.0
65.00	517.0
65.90	118.0
66.90	442.0
68.00	15387.0
69.00	15637.0
70.00	1347.0
71.90	909.0
73.00	7305.0
74.00	25944.0
75.00	76696.0
76.00	6766.0
77.00	1062.0
78.00	600.0
78.90	5360.0
79.90	1472.0
80.90	5331.0
81.90	1267.0
82.90	121.0
85.80	228.0
87.00	7050.0
87.90	6734.0
90.90	616.0
92.00	4772.0
93.00	6539.0
94.00	19216.0
95.00	149824.0
96.00	9476.0
96.90	350.0
103.90	643.0
104.80	178.0
105.90	675.0
106.90	190.0
109.80	140.0
110.90	175.0
111.90	129.0
112.80	122.0
114.80	148.0
115.90	591.0
116.80	1113.0
117.80	550.0
118.90	757.0
127.90	531.0
128.80	245.0
129.80	690.0
130.80	302.0
134.80	245.0
136.90	270.0
139.90	117.0
140.90	1586.0
141.80	220.0
142.90	1816.0
143.80	126.0
144.80	241.0
145.90	274.0
146.70	132.0
147.90	337.0
149.00	137.0
149.70	152.0
152.70	128.0
153.90	135.0
154.90	397.0
156.90	249.0
158.90	149.0
160.90	187.0
171.00	136.0
171.90	796.0
173.90	115840.0

Instrument :
MSVOA_V
ClientSampleId :
BFB215

175.00	9010.0
175.90	112680.0
176.90	7680.0
177.90	219.0

Instrument :
MSVOA_V
ClientSampleId :
BFB215

m/z	Abundance
36.00	1505.0
37.00	7344.0
38.00	6393.0
39.00	2465.0
39.90	251.0
42.90	121.0
43.90	1308.0
45.00	1403.0
46.00	191.0
47.00	2375.0
47.90	978.0
48.90	6291.0
50.00	29464.0
51.00	9314.0
51.90	534.0
55.00	440.0
56.00	2451.0
57.00	4222.0
58.10	186.0
60.00	1458.0
61.00	7446.0
62.00	6958.0
63.00	5767.0
63.90	584.0
65.00	509.0
65.90	114.0
66.90	473.0
68.00	15472.0
69.00	16072.0
70.00	1285.0
71.90	898.0
73.00	7496.0
74.00	26840.0
75.00	78064.0
76.00	6727.0
77.00	1091.0
78.00	644.0
78.90	5420.0
79.90	1493.0
80.90	5413.0
81.90	1280.0
83.00	141.0
85.80	232.0
87.00	7240.0
87.90	6948.0
90.90	605.0
92.00	4833.0
93.00	6721.0
94.00	19752.0
95.00	153280.0
96.00	9600.0
96.90	361.0
103.90	625.0
104.90	192.0
105.90	751.0
106.80	175.0
109.90	127.0
110.90	177.0
111.90	160.0
112.80	123.0
114.80	155.0
115.90	603.0
116.80	1059.0
117.90	589.0
118.90	772.0
127.80	523.0
128.80	295.0
129.80	684.0
130.80	322.0
134.80	260.0
136.90	308.0
139.90	133.0
140.90	1546.0
141.80	225.0
142.90	1758.0
143.80	126.0
144.90	271.0
145.80	283.0
146.70	135.0
147.90	358.0
148.70	120.0
149.70	150.0
152.80	124.0
153.90	113.0
154.90	436.0
156.90	240.0
158.90	147.0
160.90	171.0
170.00	105.0
171.90	777.0
173.90	122136.0
175.00	9267.0

Instrument :
MSVOA_V
ClientSampleId :
BFB215

175.90

176.90

177.90

119080.0

7833.0

212.0

Instrument :

MSVOA_V

ClientSampleId :

BFB215

m/z	Abundance
35.90	1347.0
37.00	6560.0
38.00	5641.0
39.00	2274.0
39.90	294.0
43.90	1279.0
45.00	1367.0
46.10	176.0
46.90	2116.0
47.90	961.0
48.90	5785.0
50.00	26232.0
51.00	8300.0
52.00	471.0
54.90	362.0
56.00	2149.0
57.00	3850.0
58.10	181.0
60.00	1402.0
61.00	6900.0
62.00	6424.0
63.00	5247.0
64.00	504.0
65.00	467.0
66.90	513.0
68.00	14059.0
69.00	14668.0
70.00	1142.0
71.90	791.0
73.00	6937.0
74.00	24728.0
75.00	71528.0
76.00	5916.0
77.00	947.0
78.00	592.0
78.90	4882.0
79.90	1424.0
80.90	4892.0
81.90	1154.0
83.00	146.0
85.90	262.0
87.00	6527.0
87.90	6451.0
91.00	547.0
91.90	4337.0
92.90	6187.0
94.00	17872.0
95.00	139840.0
96.00	8852.0
97.00	304.0
103.90	541.0
104.90	195.0
105.90	727.0
106.80	162.0
110.90	153.0
111.90	164.0
112.90	141.0
114.80	152.0
115.90	557.0
116.80	908.0
117.90	561.0
118.90	745.0
127.80	466.0
128.80	280.0
129.90	554.0
130.80	284.0
134.80	254.0
136.90	280.0
139.90	123.0
140.90	1392.0
141.80	186.0
142.90	1589.0
143.80	113.0
144.80	259.0
145.90	244.0
146.70	116.0
147.90	333.0
148.80	105.0
149.80	131.0
152.80	117.0
154.90	414.0
156.90	206.0
158.80	150.0
160.90	133.0
171.90	681.0
173.90	115824.0
175.00	8617.0
175.90	112816.0
176.90	7141.0
177.90	197.0

Instrument :
MSVOA_V
ClientSampleId :
BFB215