


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV100620\
 Data File : VV018683.D
 Acq On : 06 Oct 2020 09:00
 Operator : SY/MD
 Sample : BFB98
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB302

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM092320W.M
 Title : VOC Analysis
 Last Update : Wed Oct 07 05:40:49 2020

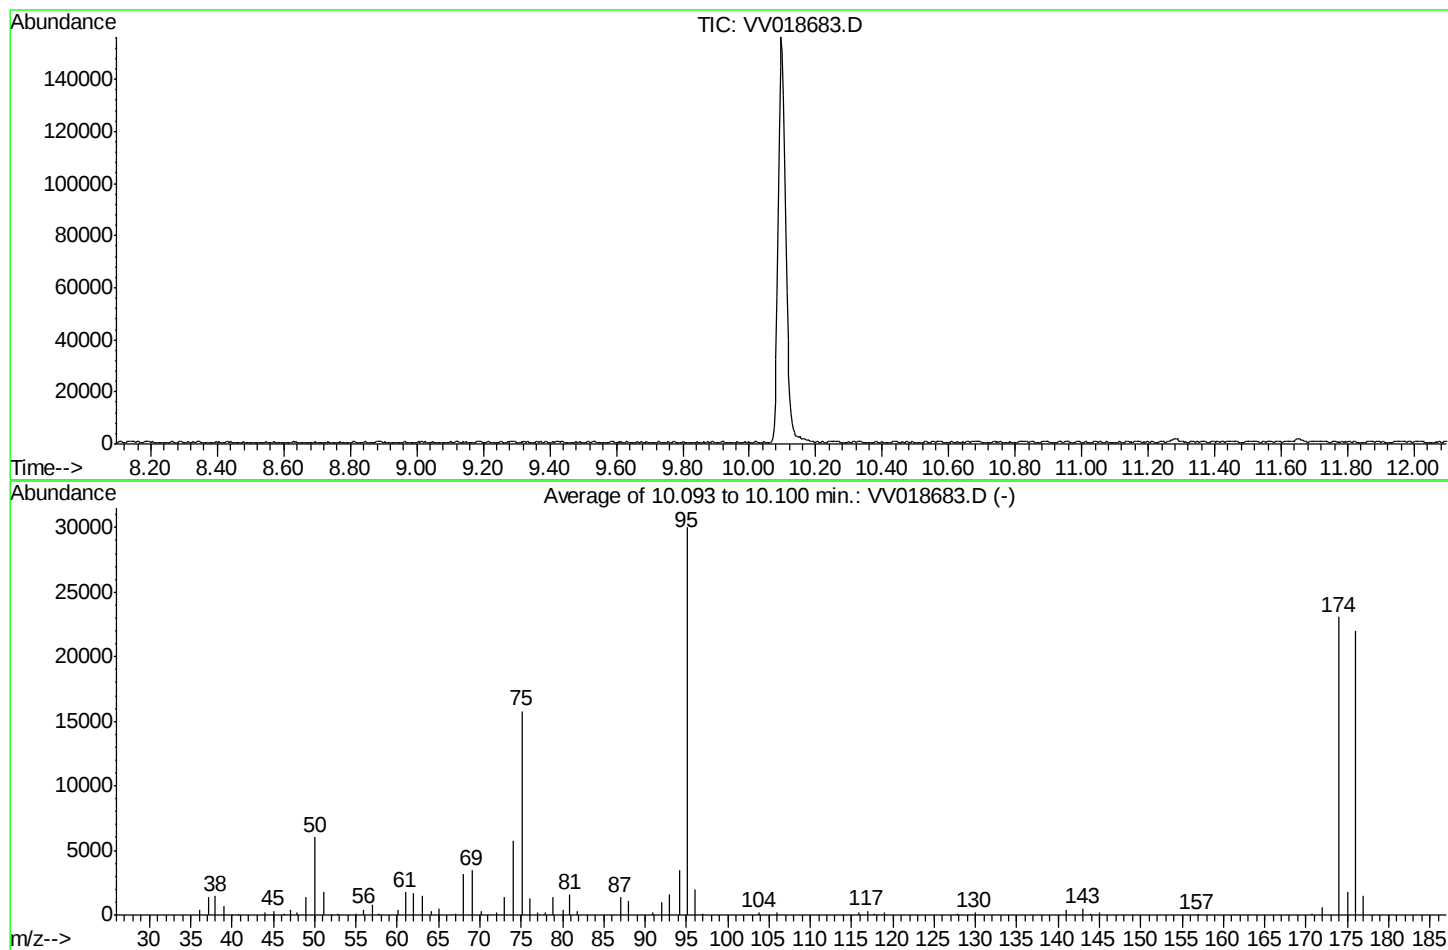

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	6022	PASS
75	95	30	80	52.6	15800	PASS
95	95	100	100	100.0	30018	PASS
96	95	5	9	6.5	1955	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.8	23061	PASS
175	174	5	9	7.7	1786	PASS
176	174	95	101	95.5	22034	PASS
177	176	5	9	6.8	1489	PASS

m/z	Abundance
36.00	506.0
37.10	1317.0
38.00	1468.0
39.00	633.0
40.00	170.0
44.00	652.0
45.00	319.0
46.30	128.0
47.00	344.0
47.90	234.0
49.00	1304.0
50.00	5974.0
51.10	1756.0
52.80	102.0
55.00	110.0
56.00	442.0
57.00	807.0
57.80	110.0
60.00	342.0
61.00	1832.0
62.00	1630.0
63.00	1464.0
64.10	257.0
65.10	450.0
67.00	137.0
68.00	3136.0
69.00	3358.0
70.10	293.0
71.90	218.0
73.00	1454.0
74.00	5557.0
75.10	15469.0
76.00	1274.0
77.00	194.0
78.10	212.0
78.90	1374.0
80.00	434.0
80.90	1496.0
81.90	267.0
87.00	1297.0
88.00	1052.0
90.90	234.0
92.00	932.0
93.00	1479.0
94.10	3372.0
95.00	28792.0
96.10	1851.0
103.90	163.0
105.90	157.0
115.80	200.0
116.90	305.0
117.80	105.0
118.90	187.0
127.80	128.0
129.90	134.0
141.00	356.0
143.00	458.0
143.90	126.0
144.90	218.0
170.70	118.0
172.00	524.0
174.00	21536.0
175.00	1696.0
176.00	21072.0
177.00	1308.0

Instrument :
MSVOA_V
ClientSampleId :
BFB302

m/z	Abundance
36.00	459.0
37.10	1498.0
38.00	1501.0
39.00	704.0
40.00	181.0
44.00	704.0
45.00	309.0
46.30	137.0
47.00	440.0
47.80	242.0
49.00	1380.0
50.00	6270.0
51.00	1855.0
52.80	106.0
54.90	135.0
56.00	430.0
57.00	797.0
57.80	115.0
60.10	408.0
61.00	1803.0
62.00	1807.0
63.10	1475.0
64.00	257.0
65.10	522.0
67.10	117.0
68.00	3230.0
69.00	3593.0
70.10	307.0
72.00	247.0
73.00	1445.0
74.00	5938.0
75.10	16342.0
76.00	1344.0
77.00	204.0
77.90	222.0
78.90	1501.0
80.00	455.0
80.90	1673.0
81.80	290.0
87.00	1417.0
87.90	1157.0
90.90	253.0
92.00	1053.0
93.00	1587.0
94.10	3576.0
95.10	31144.0
96.00	1999.0
97.00	101.0
103.90	195.0
105.90	176.0
115.80	182.0
116.90	337.0
117.80	127.0
118.90	236.0
127.80	113.0
129.70	129.0
130.00	131.0
140.90	397.0
143.00	493.0
143.90	106.0
144.90	228.0
170.70	103.0
172.00	611.0
174.00	23936.0
175.00	1843.0
176.00	22696.0
177.00	1545.0

Instrument :
MSVOA_V
ClientSampleId :
BFB302

m/z	Abundance
36.00	316.0
37.10	1496.0
38.00	1413.0
39.00	702.0
40.00	176.0
40.70	125.0
44.00	667.0
45.00	280.0
46.30	118.0
47.00	465.0
47.90	228.0
49.00	1374.0
50.10	5822.0
51.00	1767.0
52.00	113.0
54.90	160.0
55.90	394.0
57.10	709.0
60.10	397.0
61.00	1674.0
62.00	1752.0
63.10	1402.0
64.00	261.0
65.10	513.0
68.00	3067.0
69.00	3389.0
70.10	286.0
72.00	242.0
73.00	1315.0
74.00	5699.0
75.00	15591.0
76.00	1253.0
77.00	196.0
77.90	217.0
78.90	1332.0
80.00	428.0
80.90	1531.0
81.90	323.0
87.00	1360.0
87.90	1053.0
90.90	202.0
92.00	944.0
93.00	1595.0
94.10	3419.0
95.10	30120.0
96.00	2016.0
96.90	108.0
103.80	234.0
105.90	177.0
115.90	140.0
117.00	306.0
117.80	160.0
118.90	259.0
130.00	148.0
140.90	399.0
143.00	509.0
145.00	215.0
156.90	116.0
172.00	636.0
174.00	23712.0
175.10	1819.0
176.00	22336.0
177.00	1616.0

Instrument :
MSVOA_V
ClientSampleId :
BFB302

Scan 2790 (10.061 min): VV018683.D
BFB98

m/z	Abundance
40.00	160.0
42.00	106.0
44.00	450.0

Instrument :
MSVOA_V
ClientSampleId :
BFB302