

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100621\
 Data File : VW022625.D
 Acq On : 06 Oct 2021 16:37
 Operator : SY/MD
 Sample : M4051-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT3

Quant Time: Oct 07 06:18:23 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 07 06:15:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	103339	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	103214	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	47309	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	15582	4.706	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.200%
7) Chloroethane-d5	1.565	69	23194	5.197	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.000%
11) 1,1-Dichloroethene-d2	2.105	63	30803	3.206	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.200%
20) 2-Butanone-d5	3.886	46	90191	46.082	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.160%
24) Chloroform-d	4.349	84	58952	4.624	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.400%
26) 1,2-Dichloroethane-d4	5.034	65	29091	4.844	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.800%
32) Benzene-d6	5.050	84	103017	4.429	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.600%
36) 1,2-Dichloropropane-d6	6.069	67	36240	4.416	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.400%
41) Toluene-d8	7.320	98	79490	4.077	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.600%
43) trans-1,3-Dichloroprop...	7.629	79	9067	4.175	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.600%
46) 2-Hexanone-d5	8.092	63	53192	39.559	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.120%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	24352	3.906	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	78.200%
66) 1,2-Dichlorobenzene-d4	11.628	152	36907	5.043	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.800%
Target Compounds						
					Qvalue	
13) Acetone	2.175	43	3128	2.972	ug/L	# 28
14) Carbon disulfide	2.294	76	23563	1.272	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022625.D
Acq On : 06 Oct 2021 16:37
Operator : SY/MD
Sample : M4051-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT3

Quant Time: Oct 07 06:18:23 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 07 06:15:29 2021
Response via : Initial Calibration

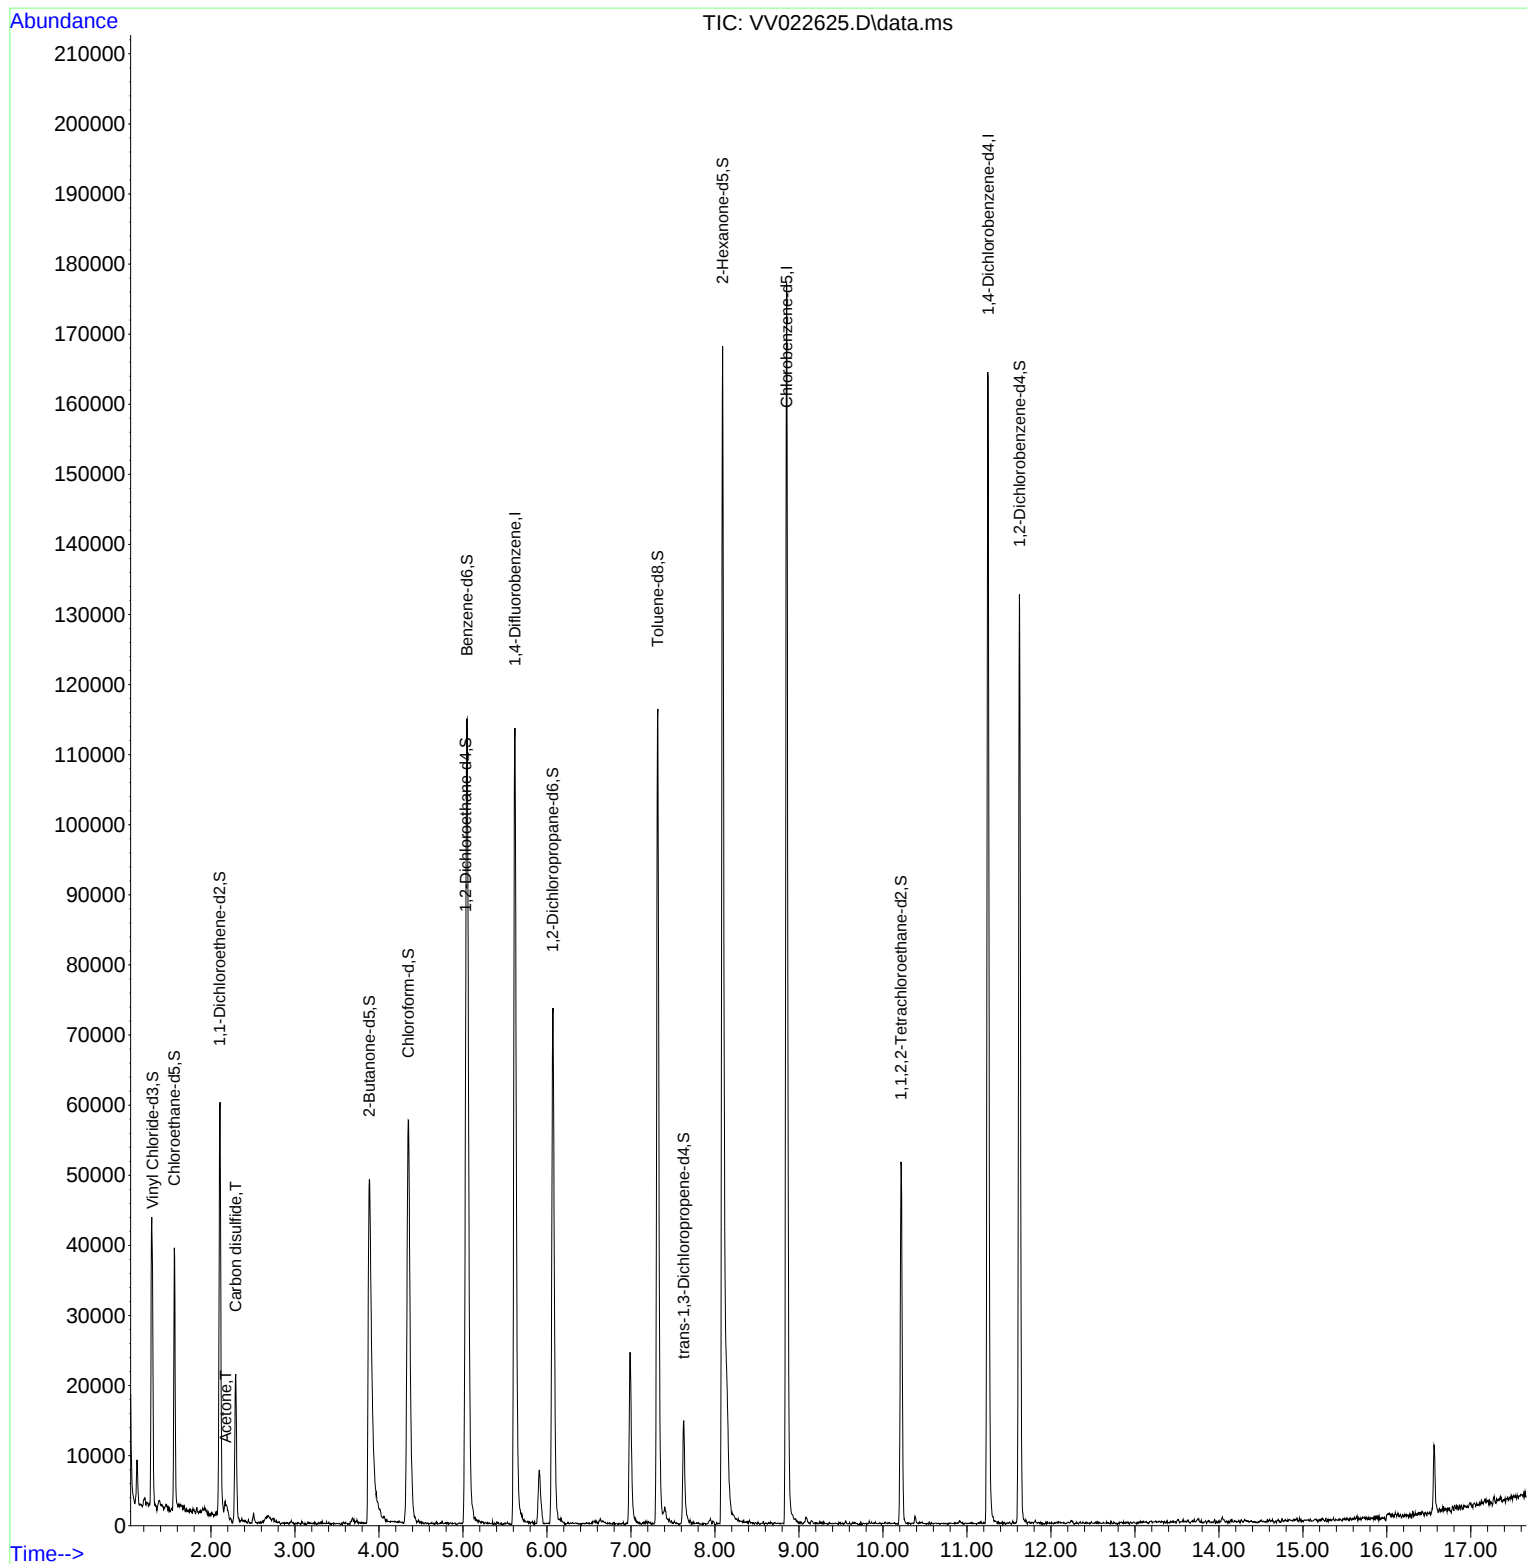

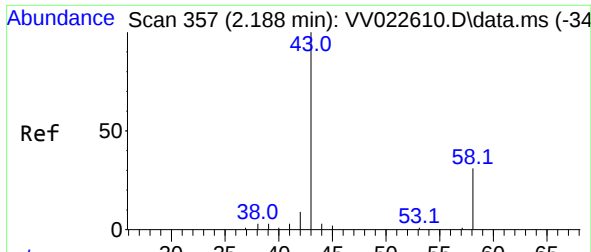

#13

Acetone

Concen: 2.972 ug/L

RT: 2.175 min Scan# 353

Delta R.T. -0.013 min

Lab File: VV022625.D





Acq: 06 Oct 2021 16:37

Tgt Ion: 43 Resp: 3128

Ion Ratio Lower Upper

43 100

58 34.8 0.0 17.6#

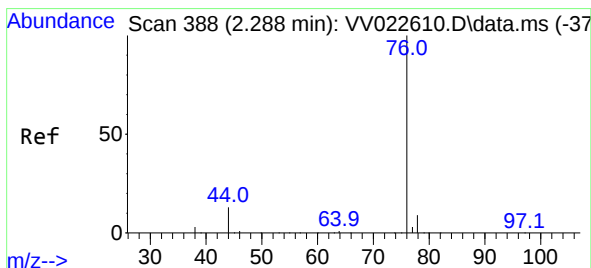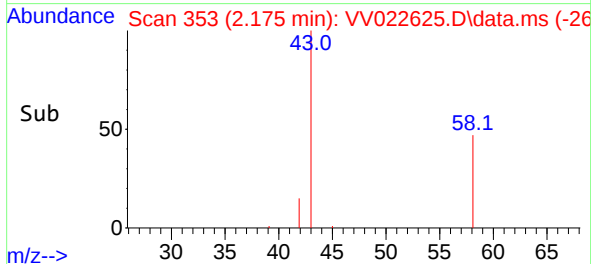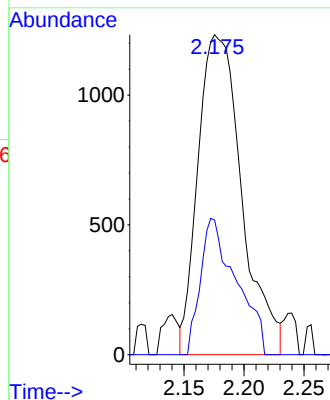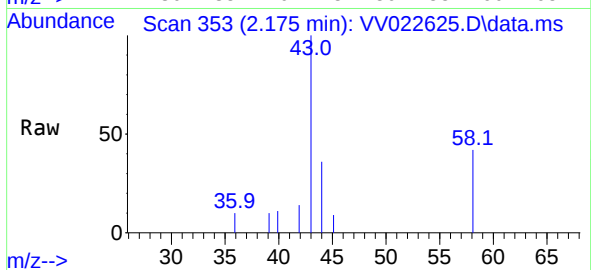

#14

Carbon disulfide

Concen: 1.272 ug/L

RT: 2.294 min Scan# 390

Delta R.T. 0.007 min

Lab File: VV022625.D

Acq: 06 Oct 2021 16:37

Tgt Ion: 76 Resp: 23563

Ion Ratio Lower Upper

76 100

78 10.1 7.8 11.6

