

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV100621\  
 Data File : VV022626.D  
 Acq On : 06 Oct 2021 17:01  
 Operator : SY/MD  
 Sample : M4051-06  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 19 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 C0AT4

Quant Time: Oct 07 06:18:31 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR100421WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Thu Oct 07 06:15:29 2021  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc     | Units  | Dev(Min) |
|-------------------------------|--------|-------|----------|----------|--------|----------|
| -----                         |        |       |          |          |        |          |
| Internal Standards            |        |       |          |          |        |          |
| 1) 1,4-Difluorobenzene        | 5.619  | 114   | 96983    | 5.000    | ug/L   | 0.00     |
| 28) Chlorobenzene-d5          | 8.853  | 117   | 96880    | 5.000    | ug/L   | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.252 | 152   | 44219    | 5.000    | ug/L   | 0.00     |
|                               |        |       |          |          |        |          |
| System Monitoring Compounds   |        |       |          |          |        |          |
| 4) Vinyl Chloride-d3          | 1.304  | 65    | 14454    | 4.652    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 40 - 130 | Recovery | =      | 93.000%  |
| 7) Chloroethane-d5            | 1.564  | 69    | 22799    | 5.443    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 130 | Recovery | =      | 108.800% |
| 11) 1,1-Dichloroethene-d2     | 2.104  | 63    | 29709    | 3.295    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 125 | Recovery | =      | 66.000%  |
| 20) 2-Butanone-d5             | 3.912  | 46    | 69878    | 38.043   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 40 - 130 | Recovery | =      | 76.080%  |
| 24) Chloroform-d              | 4.349  | 84    | 59479    | 4.971    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 99.400%  |
| 26) 1,2-Dichloroethane-d4     | 5.037  | 65    | 28962    | 5.138    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 102.800% |
| 32) Benzene-d6                | 5.047  | 84    | 104318   | 4.778    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 95.600%  |
| 36) 1,2-Dichloropropane-d6    | 6.072  | 67    | 36361    | 4.721    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 140 | Recovery | =      | 94.400%  |
| 41) Toluene-d8                | 7.316  | 98    | 78361    | 4.282    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 85.600%  |
| 43) trans-1,3-Dichloroprop... | 7.628  | 79    | 8960     | 4.396    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 55 - 130 | Recovery | =      | 88.000%  |
| 46) 2-Hexanone-d5             | 8.098  | 63    | 53346    | 42.267   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 45 - 130 | Recovery | =      | 84.540%  |
| 56) 1,1,2,2-Tetrachloroeth... | 10.220 | 84    | 25147    | 4.297    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 120 | Recovery | =      | 86.000%  |
| 66) 1,2-Dichlorobenzene-d4    | 11.628 | 152   | 36276    | 5.304    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 80 - 120 | Recovery | =      | 106.000% |
|                               |        |       |          |          |        |          |
| Target Compounds              |        |       |          |          | Qvalue |          |
| 13) Acetone                   | 2.182  | 43    | 7260     | 7.350    | ug/L   | # 60     |
| -----                         |        |       |          |          |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV100621\  
Data File : VV022626.D  
Acq On : 06 Oct 2021 17:01  
Operator : SY/MD  
Sample : M4051-06  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
C0AT4


Quant Time: Oct 07 06:18:31 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR100421WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Thu Oct 07 06:15:29 2021  
Response via : Initial Calibration

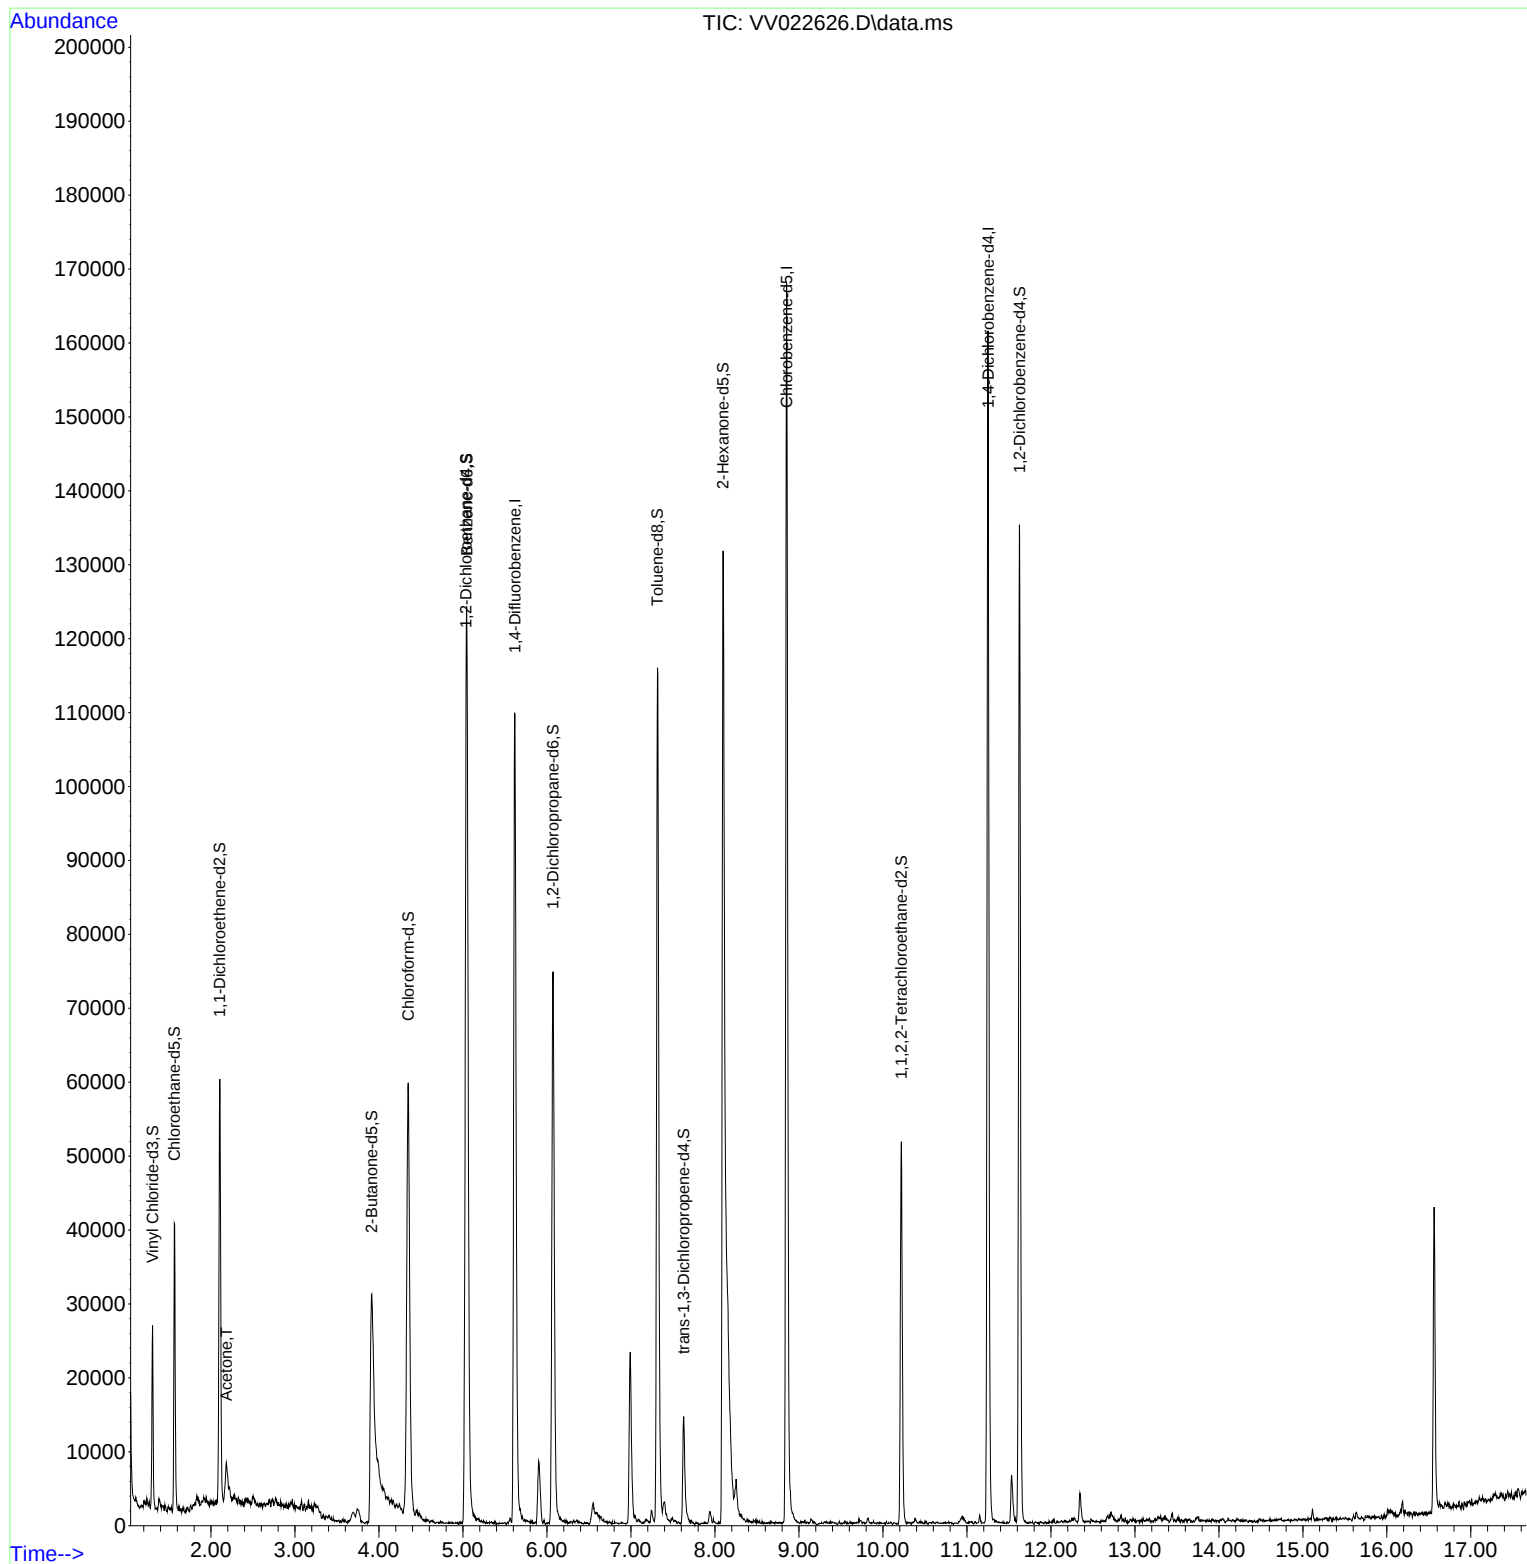

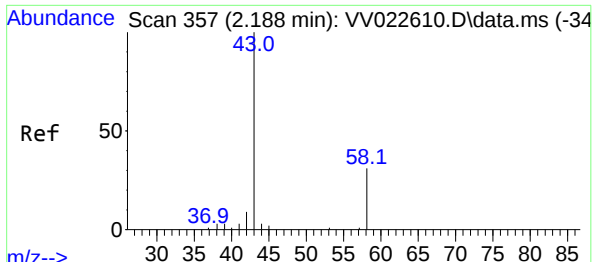

#13  
 Acetone  
 Concen: 7.350 ug/L  
 RT: 2.182 min Scan# 355  
 Delta R.T. -0.007 min  
 Lab File: VV022626.D  
 Acq: 06 Oct 2021 17:01

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 C0AT4

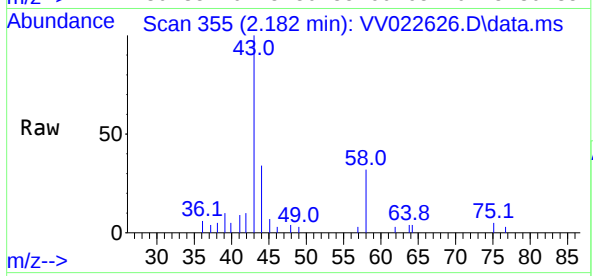

Tgt Ion: 43 Resp: 7260

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 43  | 100   |       |       |
| 58  | 23.3  | 0.0   | 17.6# |

