

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
 Data File : VV022632.D
 Acq On : 06 Oct 2021 19:26
 Operator : SY/MD
 Sample : M4050-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7B8

Quant Time: Oct 07 06:19:15 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 07 06:15:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	96740	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	96623	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	44190	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	12965	4.183	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.600%
7) Chloroethane-d5	1.565	69	20579	4.925	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.600%
11) 1,1-Dichloroethene-d2	2.105	63	27395	3.046	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.000%
20) 2-Butanone-d5	3.883	46	87357	47.679	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.360%
24) Chloroform-d	4.349	84	54394	4.557	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.200%
26) 1,2-Dichloroethane-d4	5.034	65	27883	4.959	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.200%
32) Benzene-d6	5.050	84	96733	4.443	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.800%
36) 1,2-Dichloropropane-d6	6.072	67	34427	4.481	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.600%
41) Toluene-d8	7.320	98	75114	4.115	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.400%
43) trans-1,3-Dichloroprop...	7.629	79	8638	4.249	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.000%
46) 2-Hexanone-d5	8.088	63	55990	44.480	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.960%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	25762	4.414	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	35514	5.196	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.000%
Target Compounds					Qvalue	
13) Acetone	2.175	43	3409	3.460	ug/L	# 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022632.D
Acq On : 06 Oct 2021 19:26
Operator : SY/MD
Sample : M4050-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7B8


Quant Time: Oct 07 06:19:15 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 07 06:15:29 2021
Response via : Initial Calibration

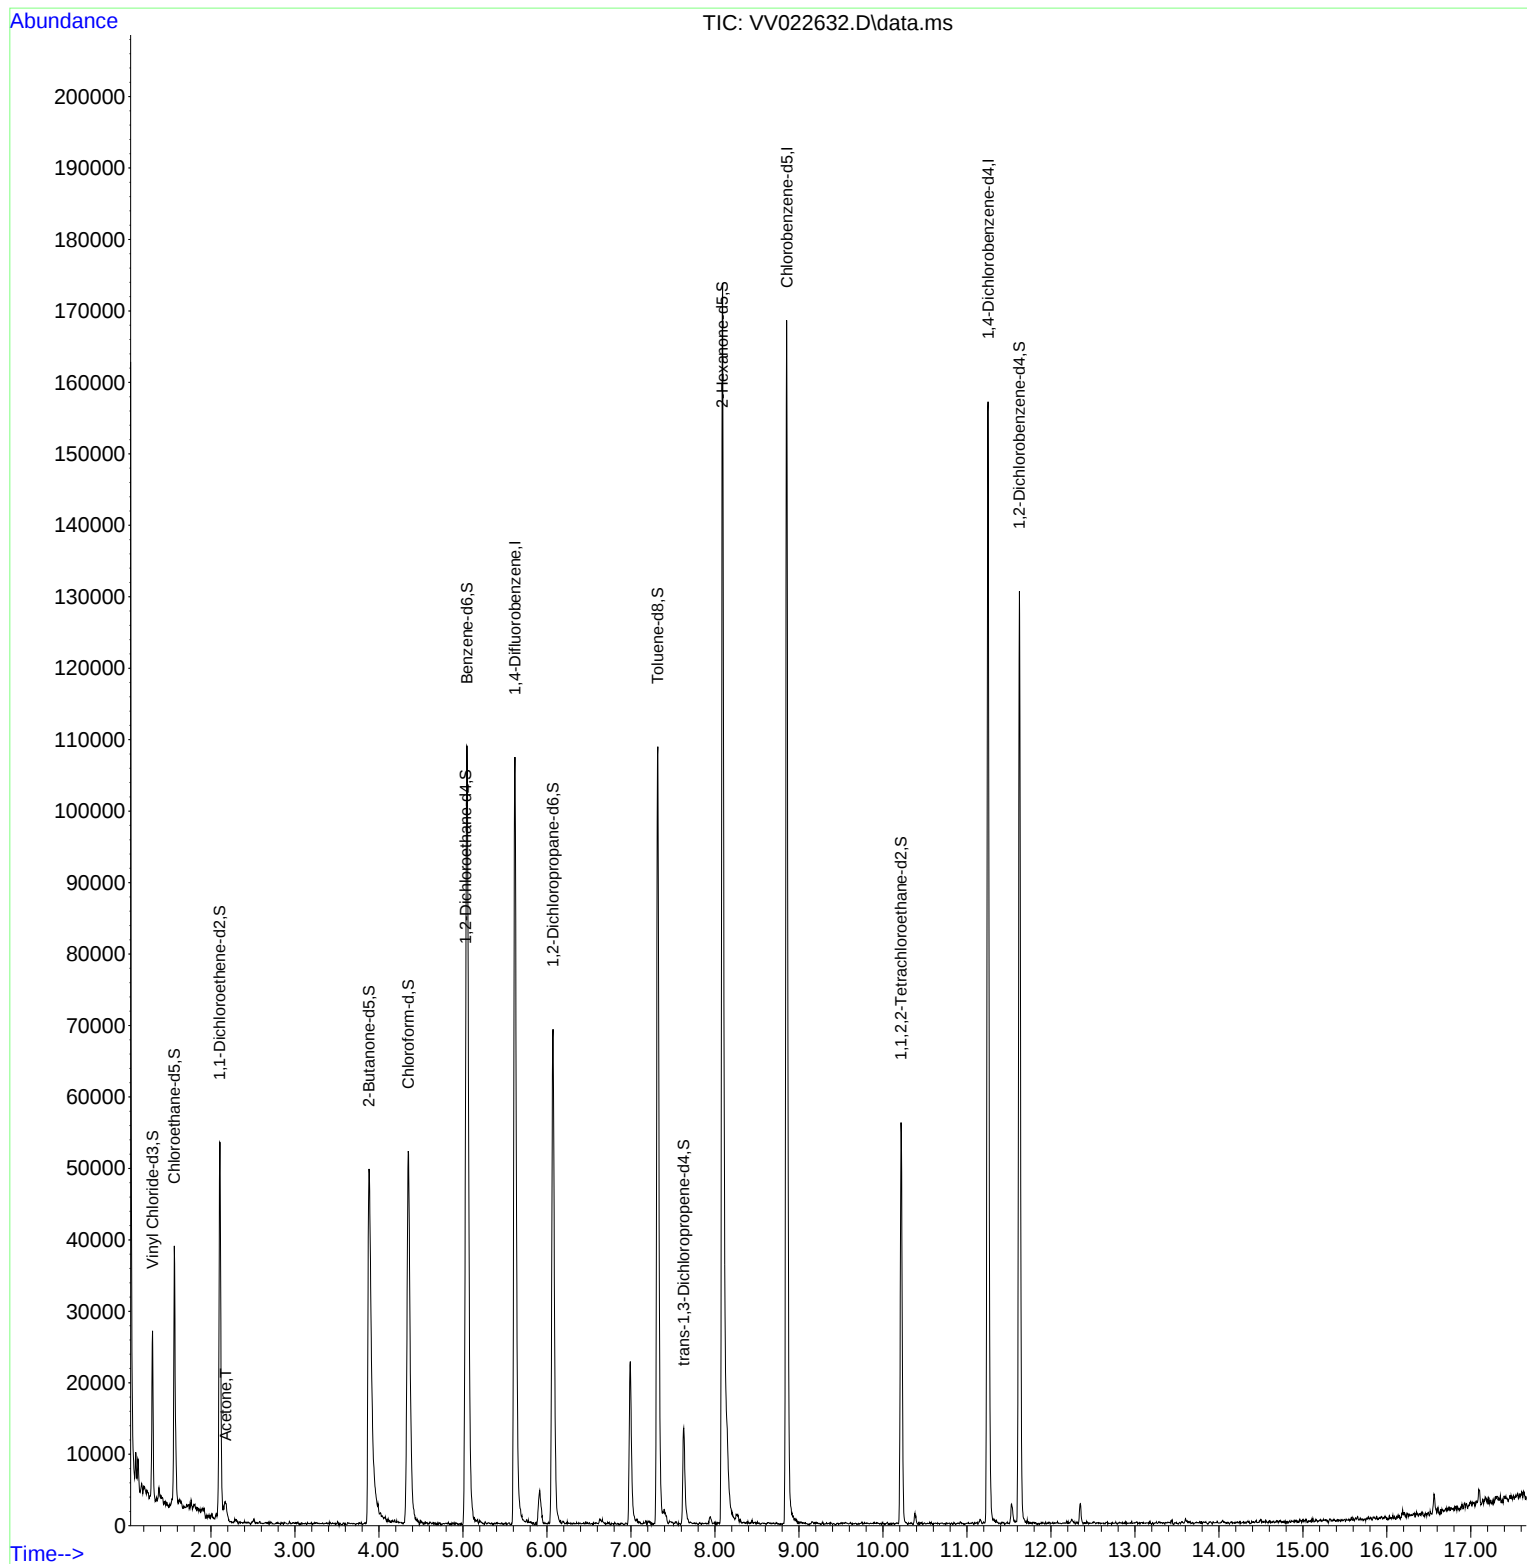

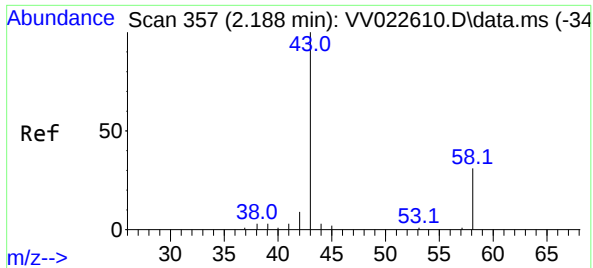

#13
 Acetone
 Concen: 3.460 ug/L
 RT: 2.175 min Scan# 353
 Delta R.T. -0.013 min
 Lab File: VV022632.D
 Acq: 06 Oct 2021 19:26

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7B8

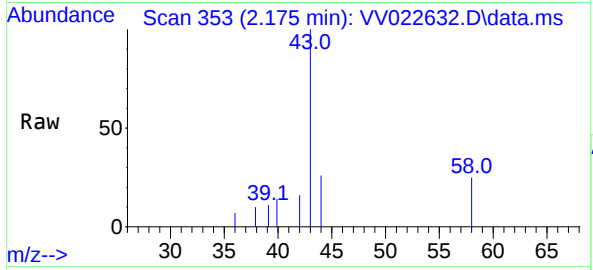

Tgt Ion: 43 Resp: 3409

Ion	Ratio	Lower	Upper
43	100		
58	20.2	0.0	17.6#

