

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100621\
 Data File : VW022641.D
 Acq On : 06 Oct 2021 23:51
 Operator : SY/MD
 Sample : M4050-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7C5

Quant Time: Oct 07 07:47:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 07 07:45:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	102507	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	101633	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	47398	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	12944	3.941	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.800%
7) Chloroethane-d5	1.564	69	20374	4.602	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.000%
11) 1,1-Dichloroethene-d2	2.108	63	26854	2.818	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	56.400%#
20) 2-Butanone-d5	3.883	46	89062	45.875	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.740%
24) Chloroform-d	4.352	84	55344	4.376	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.600%
26) 1,2-Dichloroethane-d4	5.037	65	27620	4.636	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.800%
32) Benzene-d6	5.053	84	96729	4.224	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.400%
36) 1,2-Dichloropropane-d6	6.069	67	34615	4.284	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.600%
41) Toluene-d8	7.320	98	74221	3.866	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.400%
43) trans-1,3-Dichloroprop...	7.628	79	8851	4.139	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.800%
46) 2-Hexanone-d5	8.088	63	56805	42.903	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.800%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	27067	4.409	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	35477	4.839	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.800%
Target Compounds						
					Qvalue	
13) Acetone	2.172	43	14898	14.270	ug/L #	34
14) Carbon disulfide	2.294	76	4729	0.257	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022641.D
Acq On : 06 Oct 2021 23:51
Operator : SY/MD
Sample : M4050-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7C5

Quant Time: Oct 07 07:47:37 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 07 07:45:03 2021
Response via : Initial Calibration




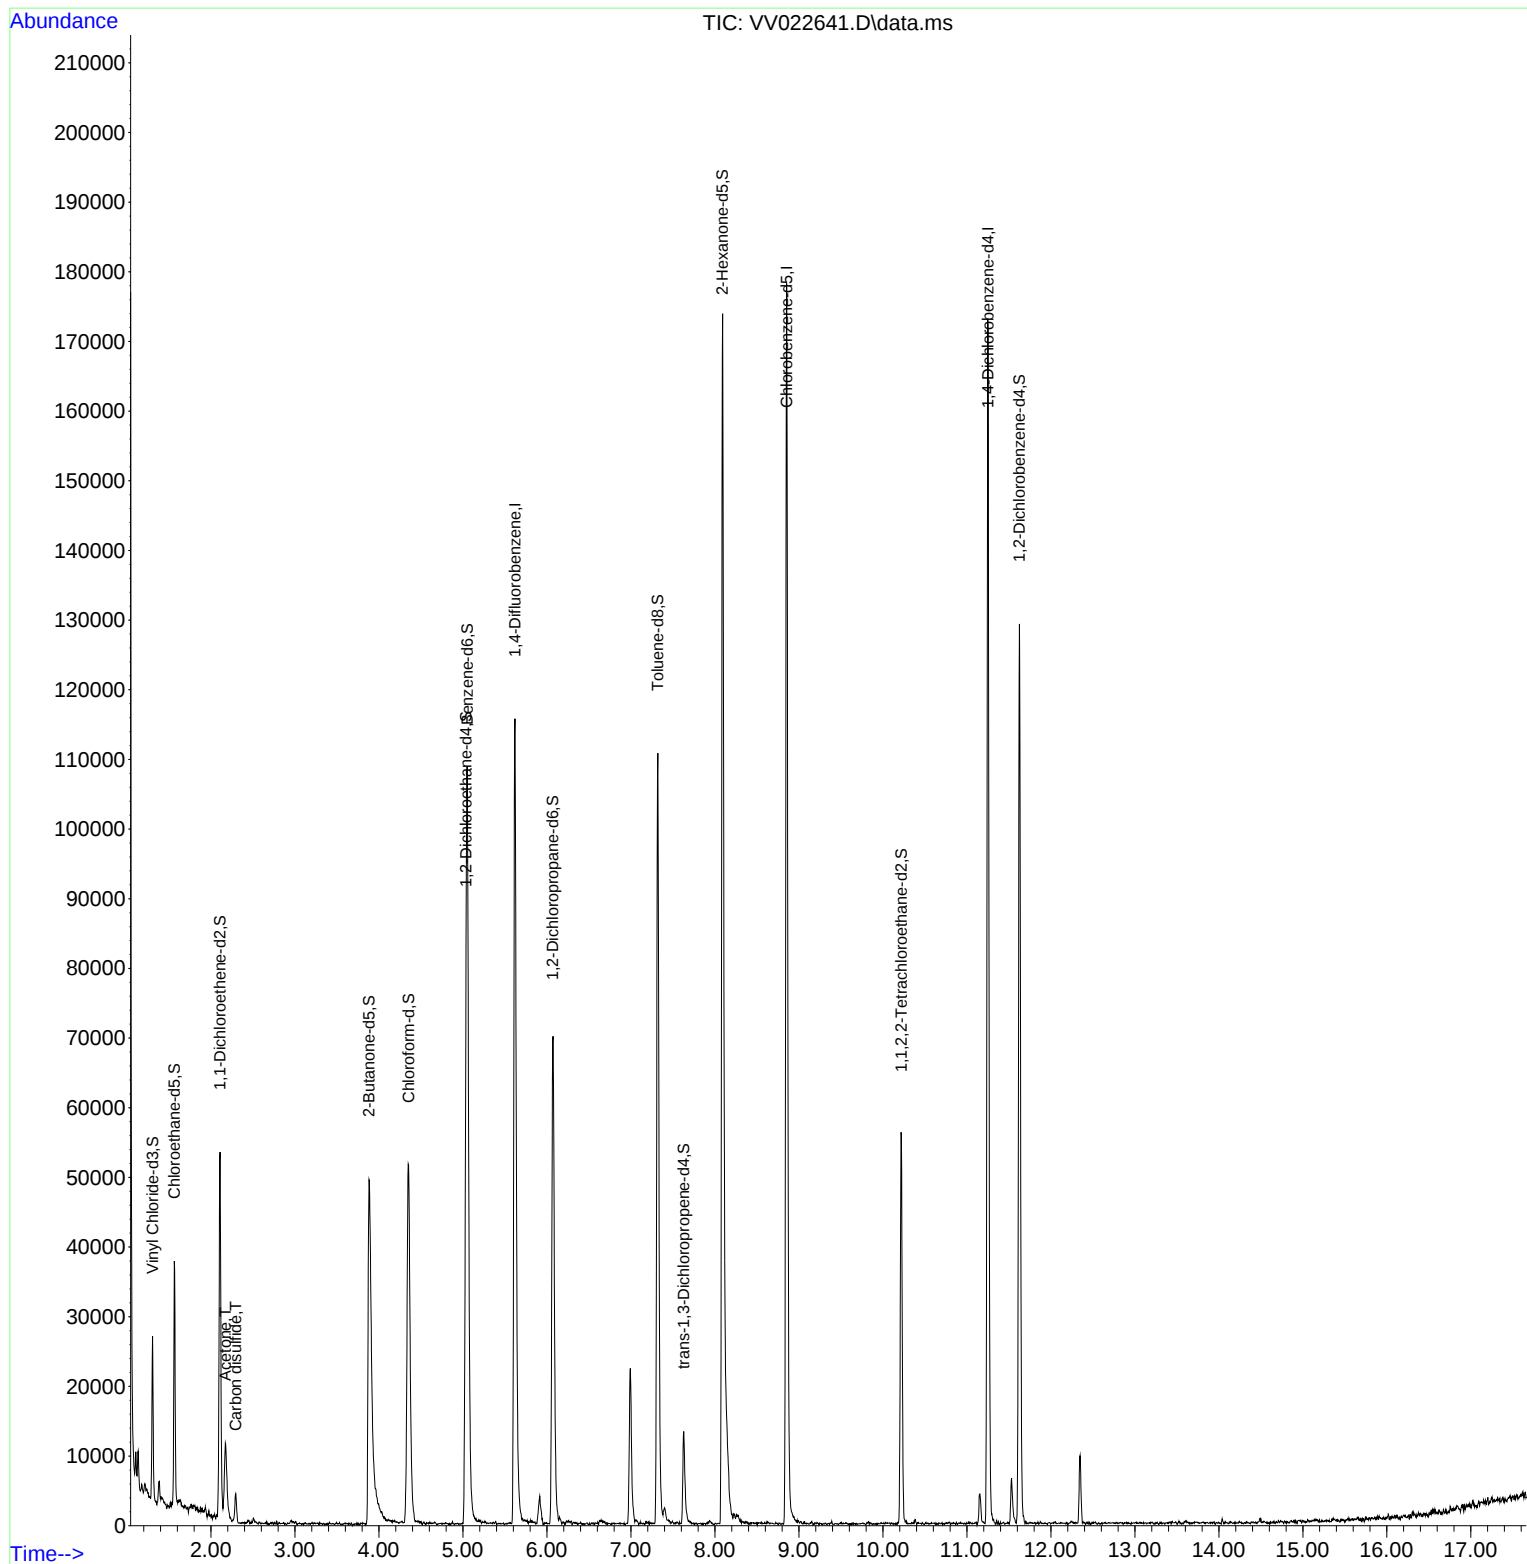


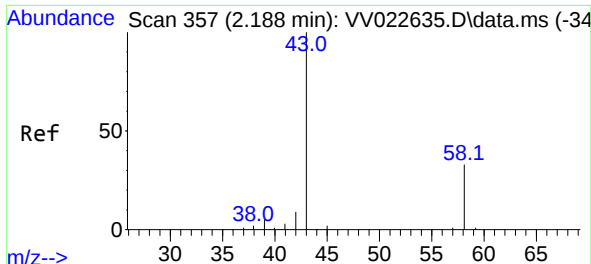

#13
Acetone
Concen: 14.270 ug/L
RT: 2.172 min Scan# 352
Delta R.T. -0.016 min
Lab File: VV022641.D
Acq: 06 Oct 2021 23:51

Instrument :
MSVOA_V
ClientSampleId :
GB7C5

Tgt Ion: 43 Resp: 14898
Ion Ratio Lower Upper
43 100
58 32.5 0.0 17.6#

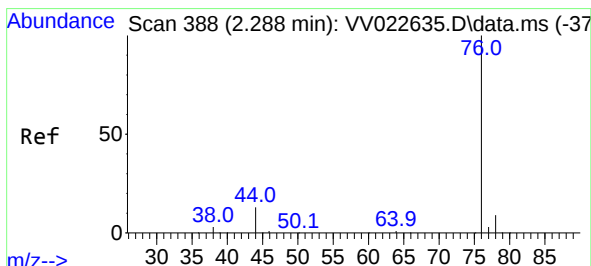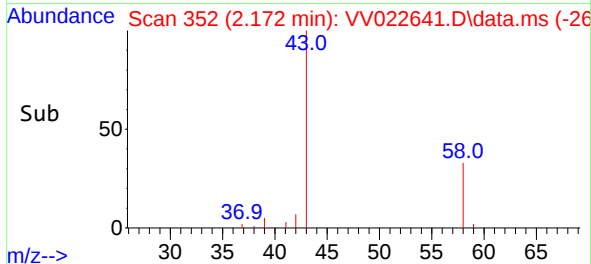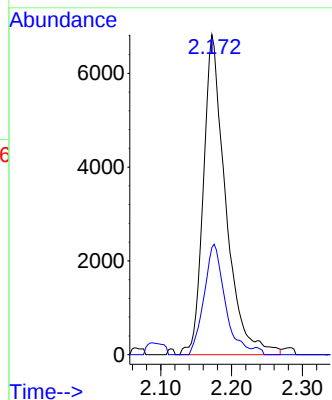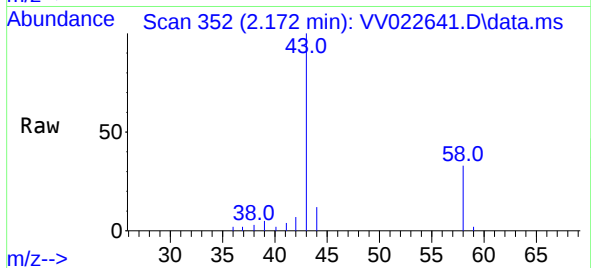

#14
Carbon disulfide
Concen: 0.257 ug/L
RT: 2.294 min Scan# 390
Delta R.T. 0.006 min
Lab File: VV022641.D
Acq: 06 Oct 2021 23:51

Tgt Ion: 76 Resp: 4729
Ion Ratio Lower Upper
76 100
78 10.7 7.8 11.6

