

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
 Data File : VV022644.D
 Acq On : 07 Oct 2021 01:03
 Operator : SY/MD
 Sample : M4050-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7C6

Quant Time: Oct 07 07:50:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 07 07:45:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	102707	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	99858	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	46573	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	13294	4.040	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.800%
7) Chloroethane-d5	1.564	69	21465	4.839	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.800%
11) 1,1-Dichloroethene-d2	2.108	63	27246	2.854	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.000%#
20) 2-Butanone-d5	3.886	46	91498	47.038	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.080%
24) Chloroform-d	4.349	84	55792	4.403	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.000%
26) 1,2-Dichloroethane-d4	5.037	65	28038	4.697	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.000%
32) Benzene-d6	5.053	84	102429	4.552	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.000%
36) 1,2-Dichloropropane-d6	6.072	67	35307	4.447	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.000%
41) Toluene-d8	7.320	98	80316	4.258	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.200%
43) trans-1,3-Dichloroprop...	7.632	79	8744	4.162	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.200%
46) 2-Hexanone-d5	8.091	63	60438	46.459	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.920%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	28242	4.682	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	38163	5.297	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.000%
Target Compounds					Qvalue	
13) Acetone	2.172	43	11492	10.986	ug/L	# 30


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022644.D
Acq On : 07 Oct 2021 01:03
Operator : SY/MD
Sample : M4050-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7C6

Quant Time: Oct 07 07:50:37 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 07 07:45:03 2021
Response via : Initial Calibration

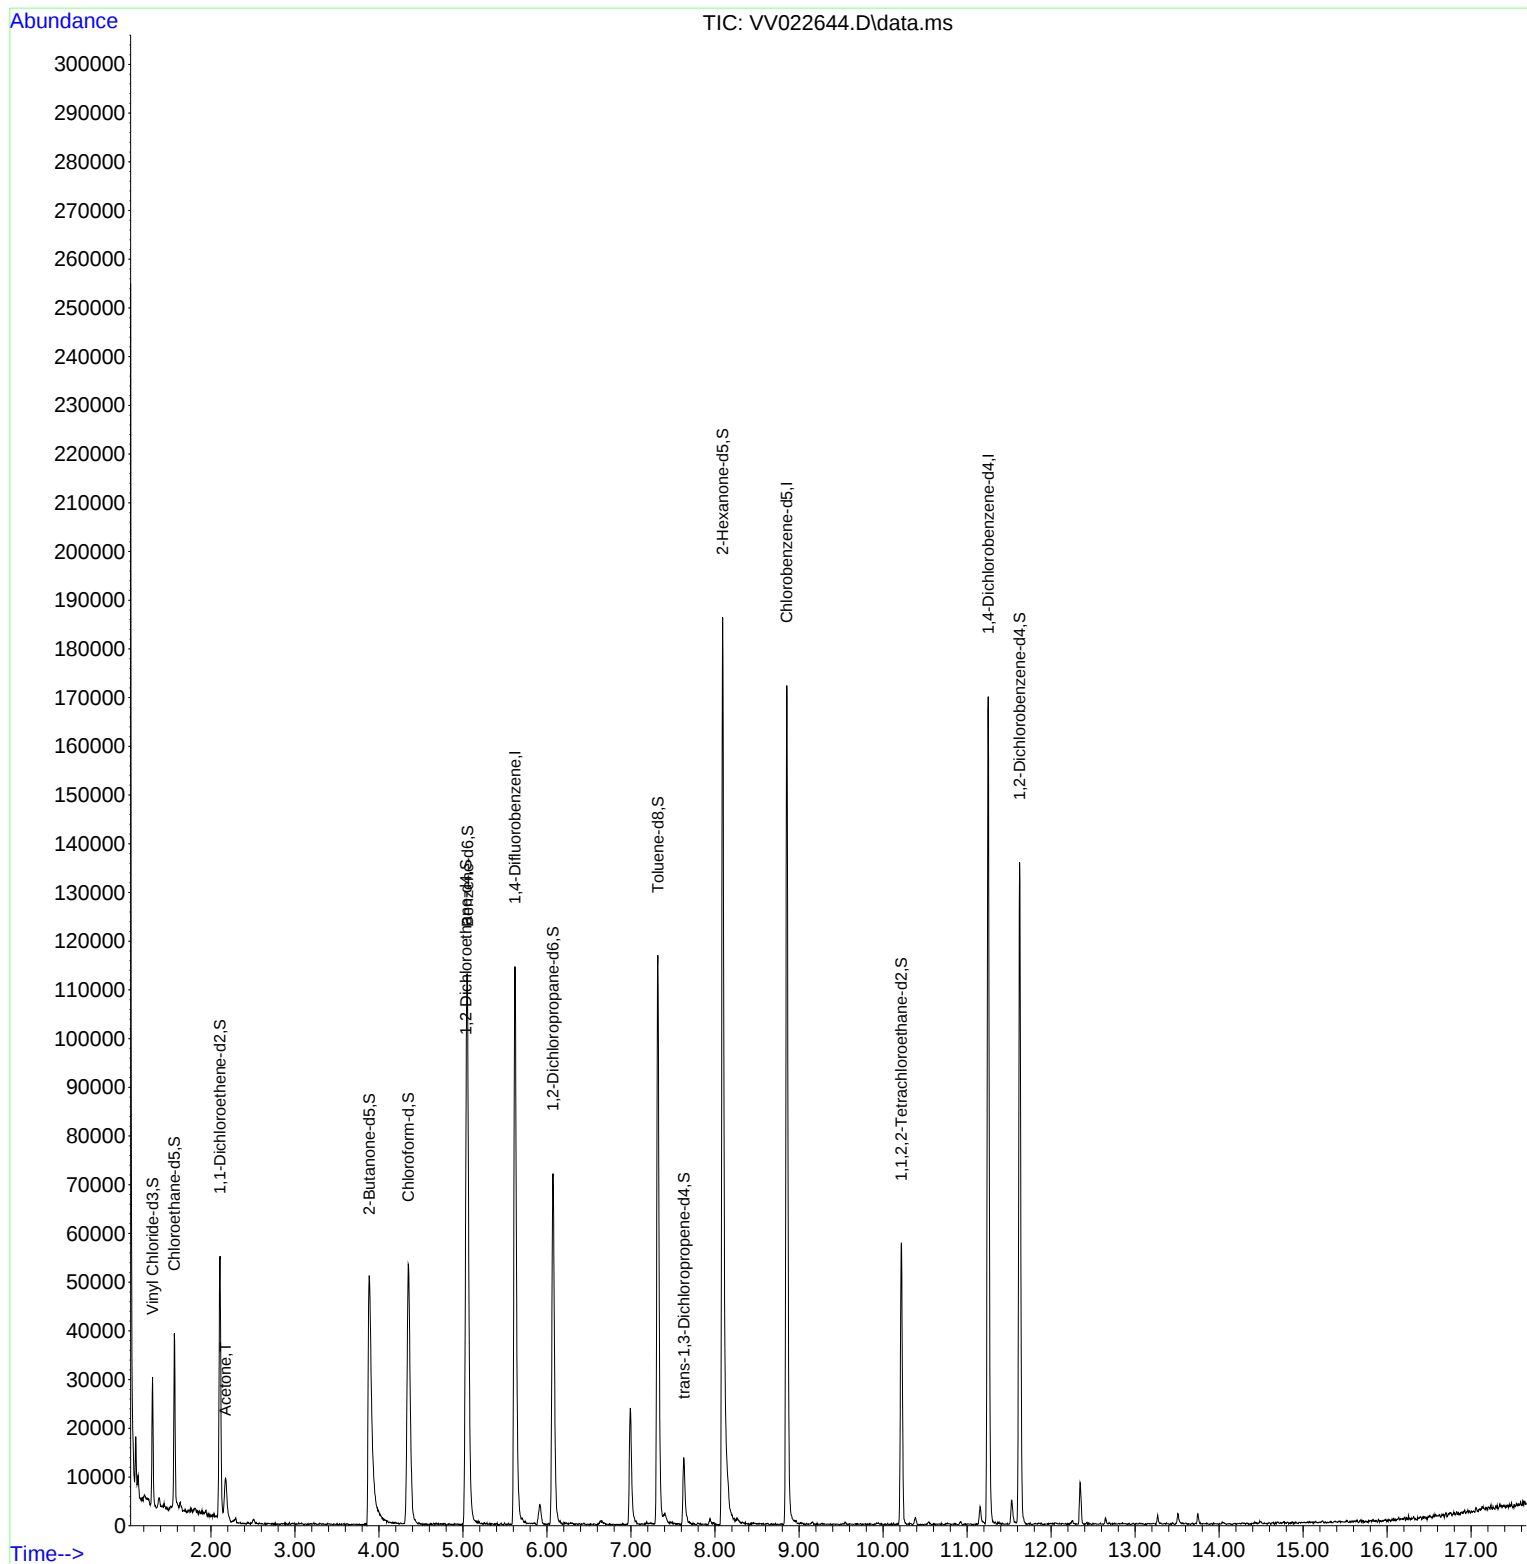

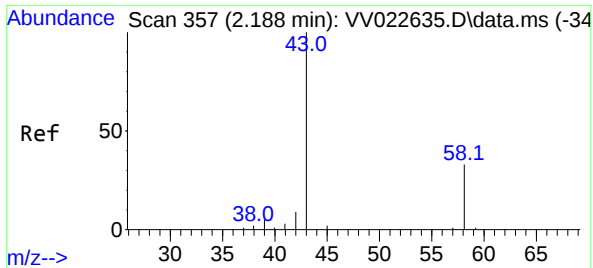

#13
Acetone
Concen: 10.986 ug/L
RT: 2.172 min Scan# 352
Delta R.T. -0.016 min
Lab File: VV022644.D
Acq: 07 Oct 2021 01:03

Instrument :
MSVOA_V
ClientSampleId :
GB7C6

Tgt Ion: 43 Resp: 11492
Ion Ratio Lower Upper
43 100
58 34.0 0.0 17.6#

