

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
 Data File : VV022612.D
 Acq On : 06 Oct 2021 11:24
 Operator : SY/MD
 Sample : M4051-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022615.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rVB	62519	62542	15.61%	1.936%
2	1.568	153	164	173	rBV	55844	66055	16.49%	2.045%
3	2.101	320	330	341	rBV	109611	156443	39.04%	4.843%
4	2.500	445	454	462	rBV3	5291	9117	2.28%	0.282%
5	3.027	608	618	626	rBV3	3440	5733	1.43%	0.177%
6	3.918	883	895	927	rBV2	28837	112390	28.05%	3.479%
7	4.342	1012	1027	1052	rVB2	71290	181265	45.24%	5.611%
8	5.040	1228	1244	1266	rBV2	171157	400679	100.00%	12.403%
9	5.616	1407	1423	1443	rBV	128422	260235	64.95%	8.055%
10	5.905	1502	1513	1526	rBV6	6533	14338	3.58%	0.444%
11	6.069	1550	1564	1583	rBV	89486	185585	46.32%	5.745%
12	6.989	1840	1850	1870	rBV2	35185	65677	16.39%	2.033%
13	7.317	1941	1952	1968	rBV	183562	323569	80.76%	10.016%
14	7.390	1971	1975	1986	rVB4	4353	7413	1.85%	0.229%
15	7.625	2034	2048	2069	rBV	20402	37631	9.39%	1.165%
16	7.979	2150	2158	2166	rVB6	4407	6865	1.71%	0.213%
17	8.098	2182	2195	2234	rBV2	135147	351590	87.75%	10.883%
18	8.853	2418	2430	2450	rBV	192095	318709	79.54%	9.866%
19	10.220	2843	2855	2870	rBV2	59812	97151	24.25%	3.007%
20	11.252	3164	3176	3194	rBV	184015	288164	71.92%	8.920%
21	11.625	3281	3292	3311	rBV	179411	279385	69.73%	8.648%




Sum of corrected areas: 3230536

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022612.D
Acq On : 06 Oct 2021 11:24
Operator : SY/MD
Sample : M4051-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

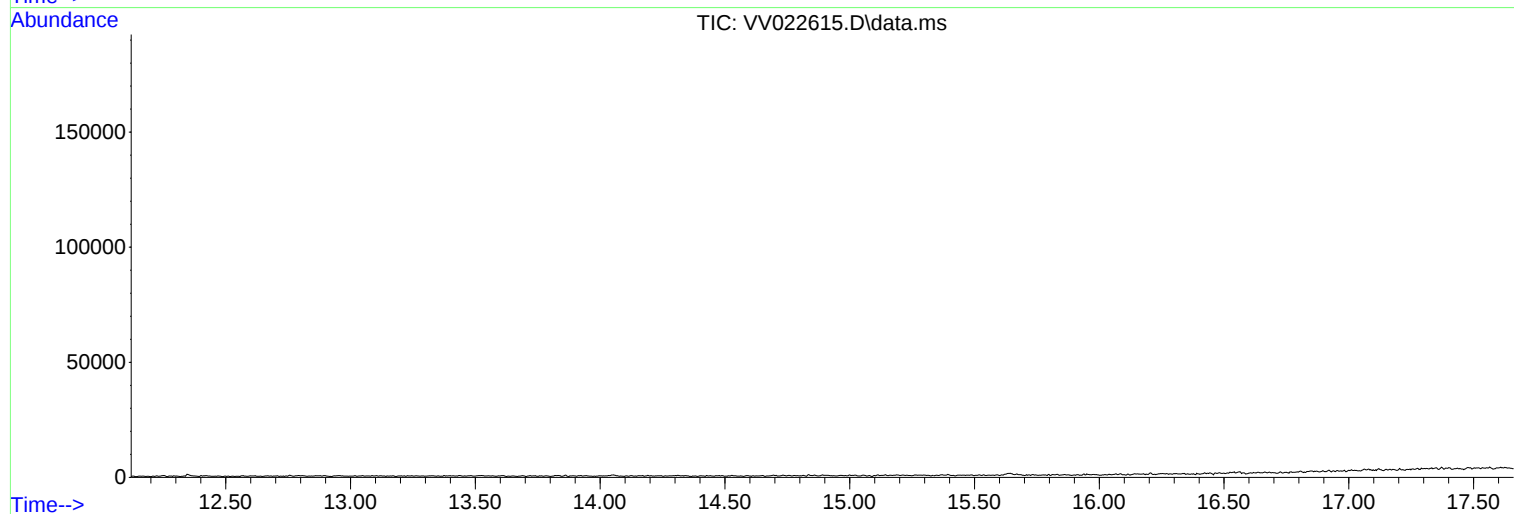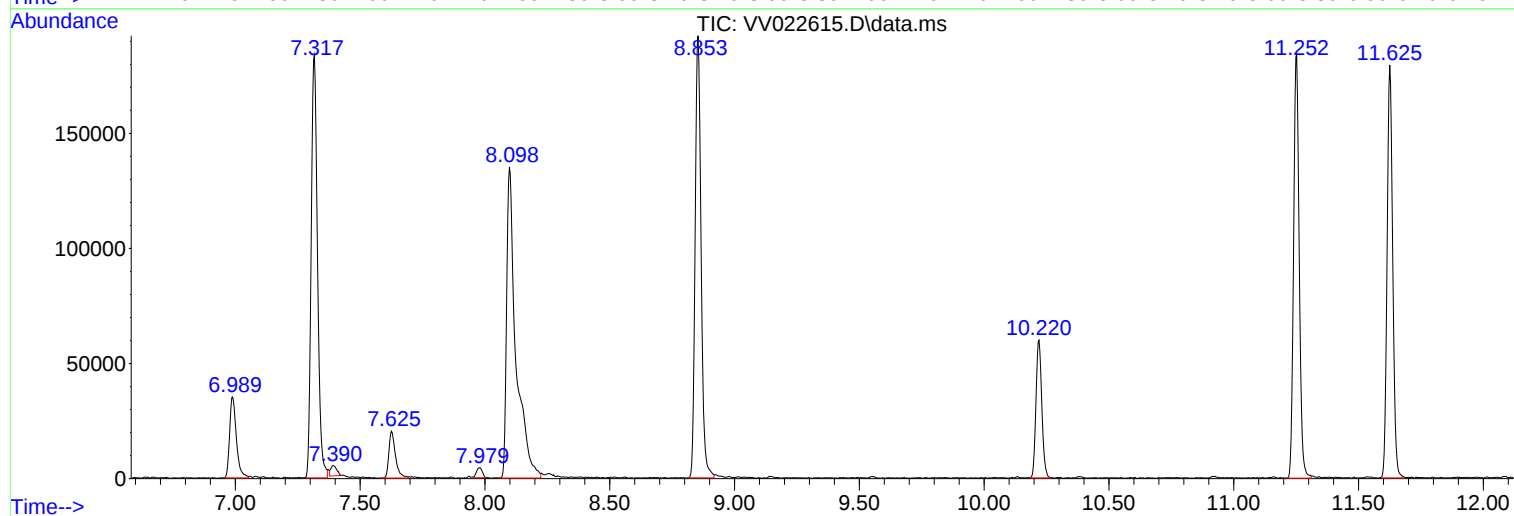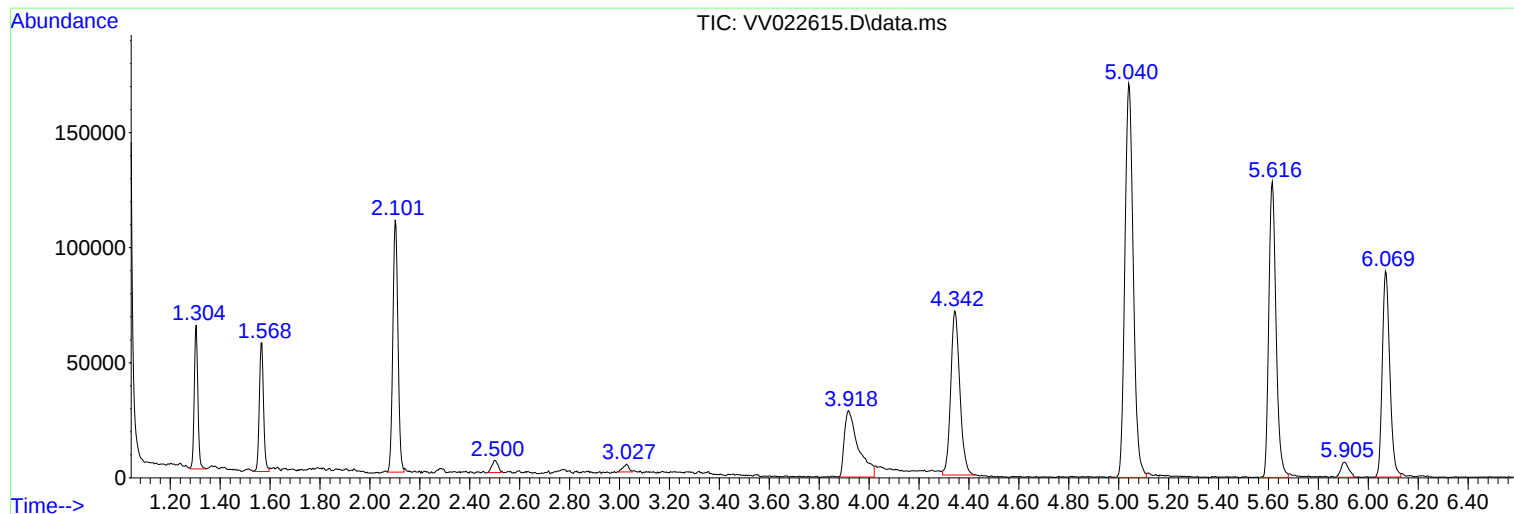

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022612.D
Acq On : 06 Oct 2021 11:24
Operator : SY/MD
Sample : M4051-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022612.D
Acq On : 06 Oct 2021 11:24
Operator : SY/MD
Sample : M4051-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
