

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
 Data File : VV022613.D
 Acq On : 06 Oct 2021 11:48
 Operator : SY/MD
 Sample : M4051-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022616.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rBV	64051	62944	13.95%	1.711%
2	1.564	156	163	174	rBV	55753	64137	14.21%	1.743%
3	2.105	319	331	349	rBV	112056	168988	37.45%	4.594%
4	3.912	880	893	928	rBV4	47479	171230	37.94%	4.655%
5	4.352	1013	1030	1058	rBV2	67256	180508	40.00%	4.907%
6	4.831	1168	1179	1189	rBV4	2680	5689	1.26%	0.155%
7	5.050	1230	1247	1271	rBV2	153866	384170	85.13%	10.443%
8	5.619	1412	1424	1447	rBV	119355	248280	55.02%	6.749%
9	5.915	1502	1516	1548	rBV	225639	451294	100.00%	12.268%
10	6.072	1553	1565	1586	rBV2	87492	182810	40.51%	4.969%
11	6.989	1839	1850	1871	rBV	34348	64759	14.35%	1.760%
12	7.317	1941	1952	1972	rBV	179168	316618	70.16%	8.607%
13	7.397	1974	1977	1988	rVB3	2682	4533	1.00%	0.123%
14	7.625	2037	2048	2069	rBV2	20392	37906	8.40%	1.030%
15	7.979	2150	2158	2168	rVB4	11522	19004	4.21%	0.517%
16	8.095	2183	2194	2229	rBV2	154035	361400	80.08%	9.824%
17	8.854	2420	2430	2450	rBV	187626	309844	68.66%	8.422%
18	10.220	2844	2855	2868	rBV	60056	96229	21.32%	2.616%
19	11.249	3164	3175	3197	rBV	176363	276717	61.32%	7.522%
20	11.625	3281	3292	3308	rBV	171113	271714	60.21%	7.386%




Sum of corrected areas: 3678774

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022613.D
Acq On : 06 Oct 2021 11:48
Operator : SY/MD
Sample : M4051-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0AW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

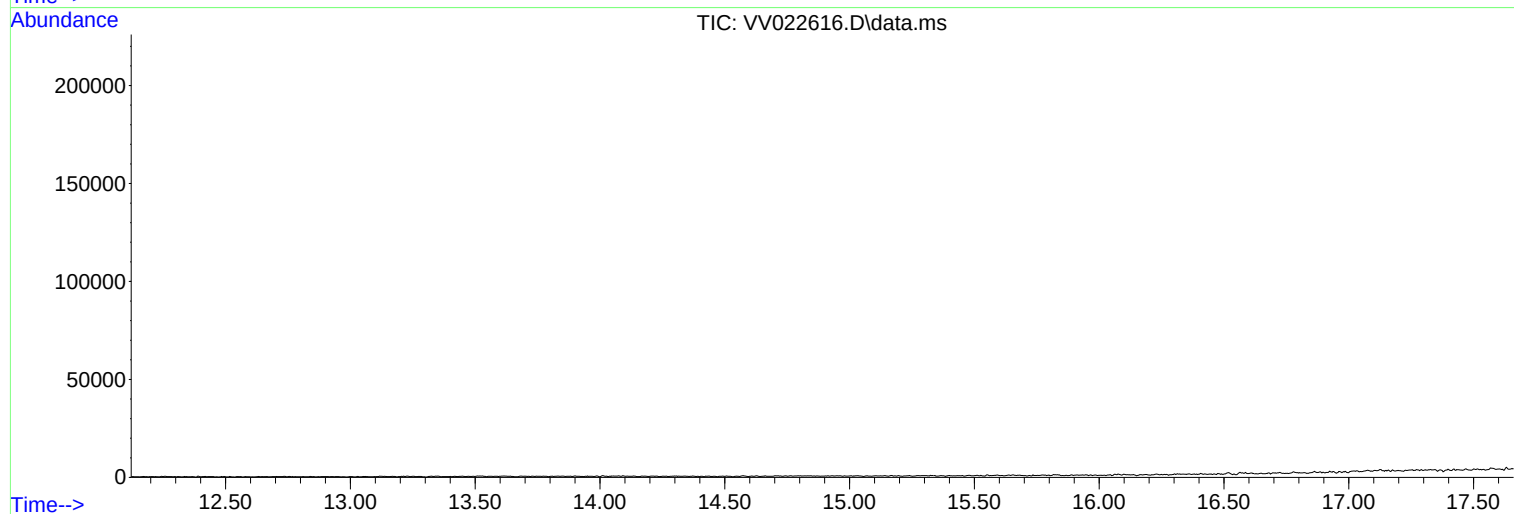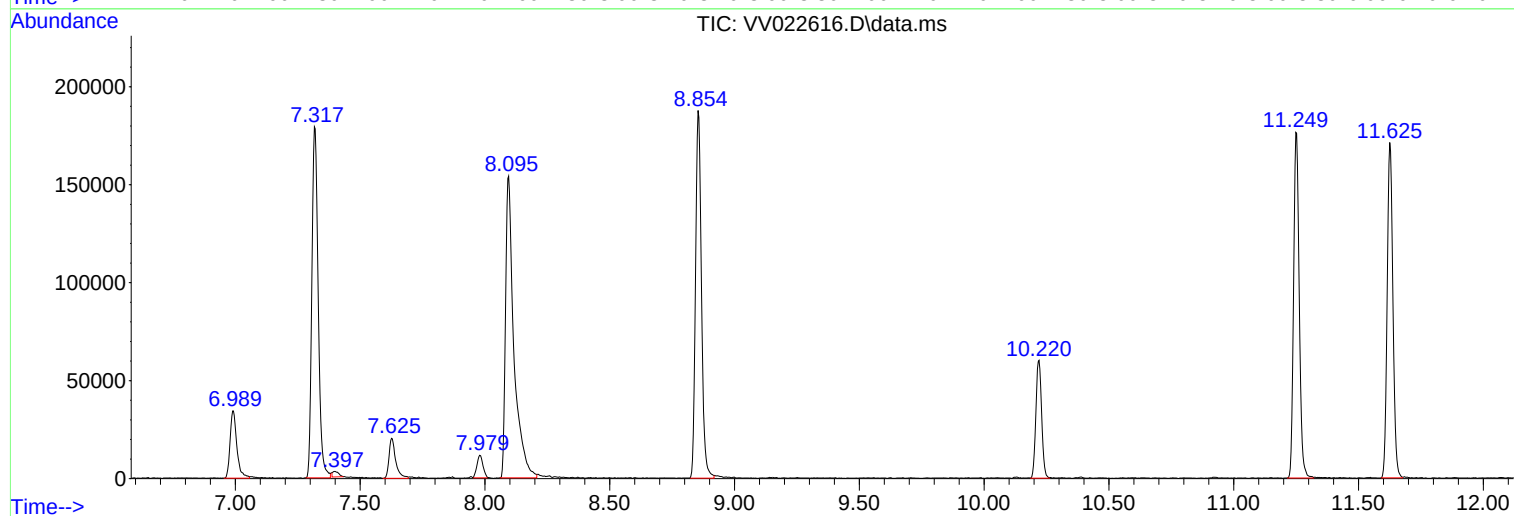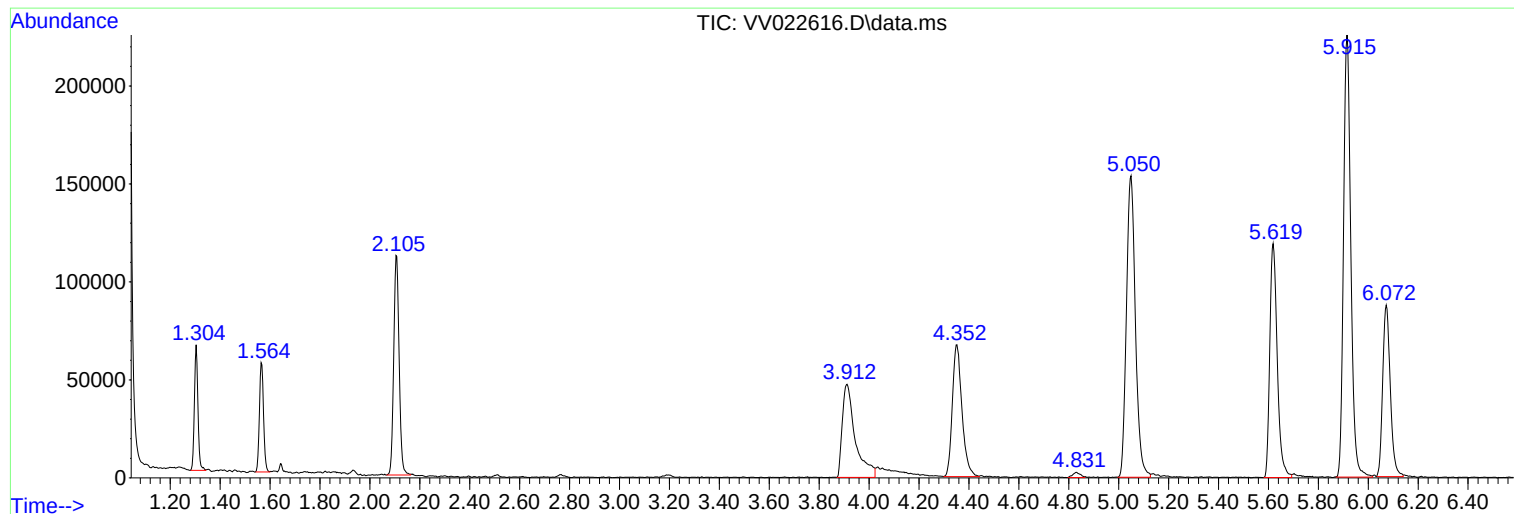

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022613.D
Acq On : 06 Oct 2021 11:48
Operator : SY/MD
Sample : M4051-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022613.D
Acq On : 06 Oct 2021 11:48
Operator : SY/MD
Sample : M4051-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
