

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
 Data File : VV022614.D
 Acq On : 06 Oct 2021 12:12
 Operator : SY/MD
 Sample : M4051-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022617.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	30903	33448	10.08%	1.240%
2	1.568	158	164	170	rBV	37199	39006	11.75%	1.446%
3	2.108	324	332	349	rVB	76384	137102	41.31%	5.084%
4	2.294	380	390	401	rBV	4628	7566	2.28%	0.281%
5	2.510	447	457	469	rVB5	3471	6259	1.89%	0.232%
6	3.883	874	884	920	rBV	50439	152371	45.92%	5.650%
7	4.352	1014	1030	1051	rBV2	56402	142098	42.82%	5.269%
8	5.050	1231	1247	1277	rBV4	114410	289700	87.30%	10.743%
9	5.619	1412	1424	1446	rBV	115073	234654	70.71%	8.702%
10	5.918	1504	1517	1540	rVB7	16729	37515	11.30%	1.391%
11	6.072	1548	1565	1587	rBV	73478	149740	45.12%	5.553%
12	6.992	1841	1851	1866	rBV2	21730	40928	12.33%	1.518%
13	7.320	1940	1953	1970	rBV	117032	205195	61.83%	7.609%
14	7.397	1970	1977	1994	rVB2	4269	8461	2.55%	0.314%
15	7.628	2039	2049	2063	rBV2	12955	22471	6.77%	0.833%
16	8.091	2183	2193	2229	rBV2	149988	331853	100.00%	12.306%
17	8.853	2417	2430	2456	rBV	178213	292996	88.29%	10.865%
18	10.217	2844	2854	2874	rVB	53434	84599	25.49%	3.137%
19	11.252	3165	3176	3195	rBV	168312	269434	81.19%	9.991%
20	11.625	3280	3292	3311	rBV	128814	207487	62.52%	7.694%
21	12.348	3510	3517	3525	rVB4	2982	3793	1.14%	0.141%




Sum of corrected areas: 2696676

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022614.D
Acq On : 06 Oct 2021 12:12
Operator : SY/MD
Sample : M4051-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

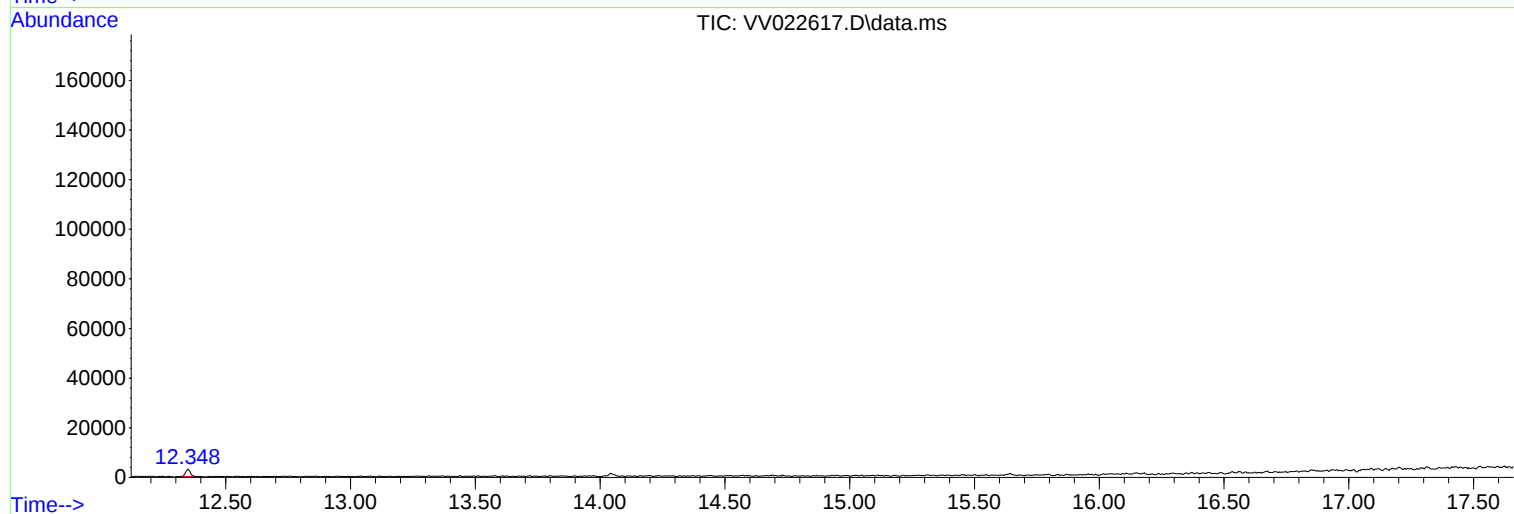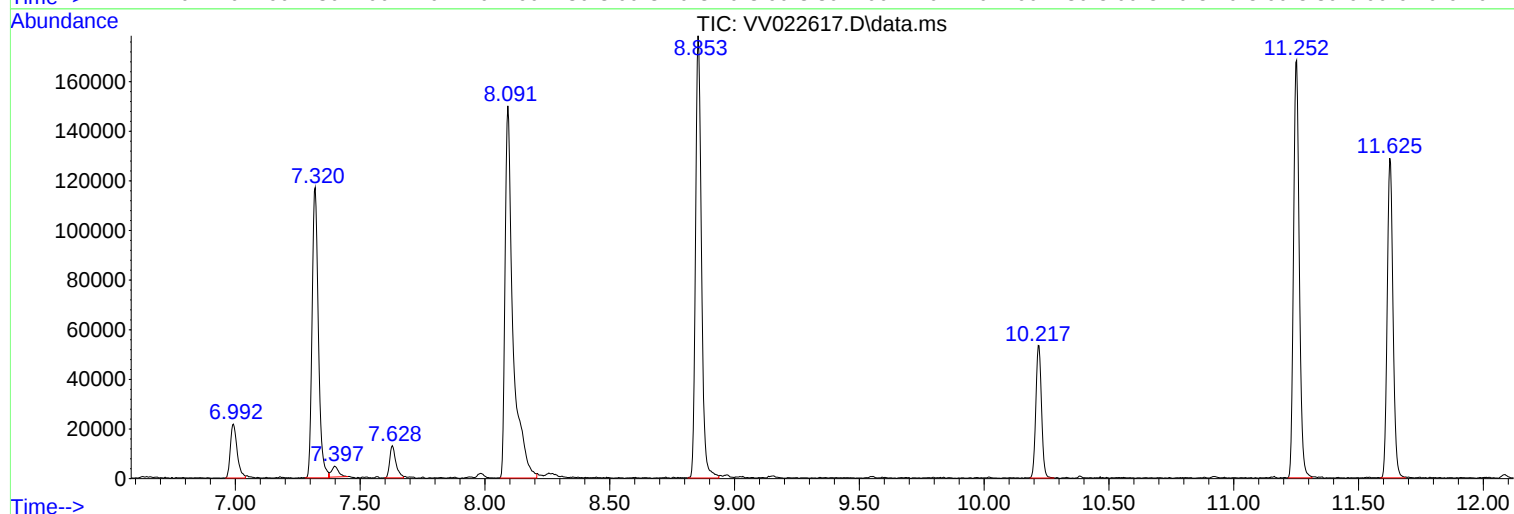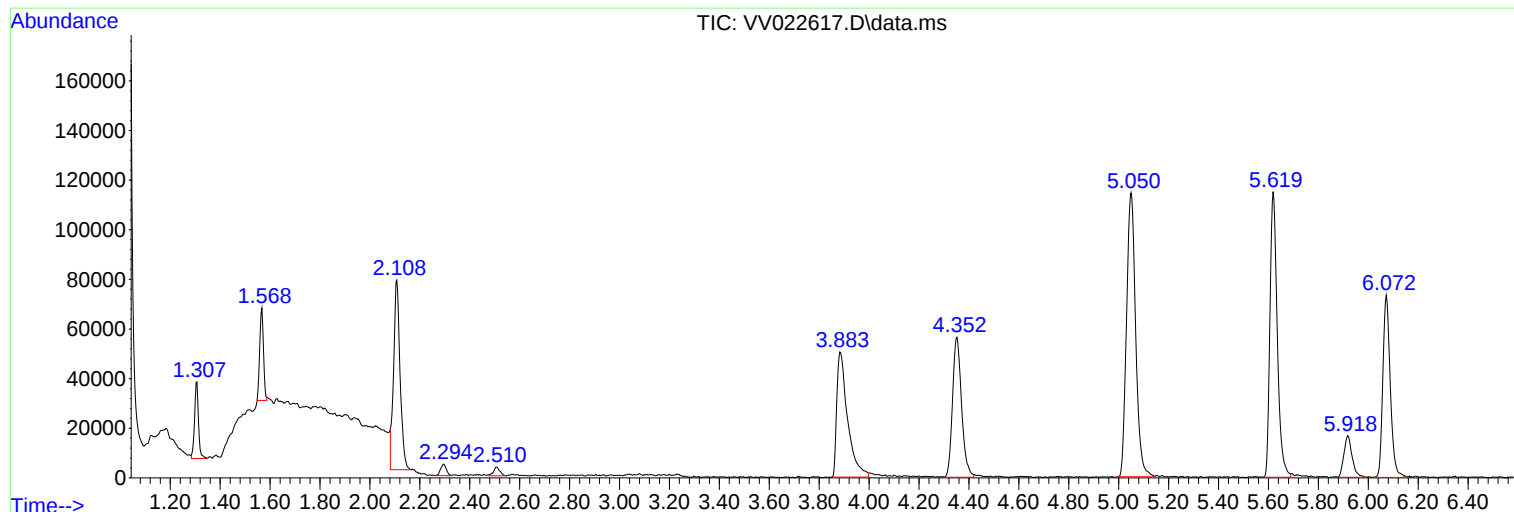

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022614.D
Acq On : 06 Oct 2021 12:12
Operator : SY/MD
Sample : M4051-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022614.D
Acq On : 06 Oct 2021 12:12
Operator : SY/MD
Sample : M4051-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
