

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
 Data File : VV022616.D
 Acq On : 06 Oct 2021 13:00
 Operator : SY/MD
 Sample : M4051-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022619.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	93	rVB	62549	61553	15.78%	1.806%
2	1.565	156	163	172	rBV	58698	64489	16.54%	1.892%
3	2.108	321	332	350	rVB3	133440	216587	55.53%	6.355%
4	3.908	881	892	920	rBV2	27907	106353	27.27%	3.121%
5	4.349	1011	1029	1058	rVB2	69854	178458	45.76%	5.237%
6	4.825	1165	1177	1180	rBV2	3350	4964	1.27%	0.146%
7	5.050	1228	1247	1272	rBV3	156741	390013	100.00%	11.444%
8	5.619	1409	1424	1442	rBV	119323	242591	62.20%	7.118%
9	5.915	1503	1516	1545	rVB4	55668	115698	29.67%	3.395%
10	6.072	1549	1565	1583	rBV	87983	181766	46.61%	5.334%
11	6.989	1840	1850	1871	rBV2	33423	63372	16.25%	1.860%
12	7.317	1939	1952	1969	rBV	180711	319935	82.03%	9.388%
13	7.400	1974	1978	1996	rVB7	2819	5351	1.37%	0.157%
14	7.629	2040	2049	2066	rBV2	18718	33018	8.47%	0.969%
15	7.979	2137	2158	2173	rBV2	65182	113552	29.11%	3.332%
16	8.095	2181	2194	2233	rBV2	147023	351768	90.19%	10.322%
17	8.854	2420	2430	2455	rBV	184980	305651	78.37%	8.969%
18	10.220	2843	2855	2872	rBV2	62167	99500	25.51%	2.920%
19	11.252	3165	3176	3201	rBV	173650	275549	70.65%	8.086%
20	11.625	3281	3292	3309	rBV	173952	277748	71.22%	8.150%




Sum of corrected areas: 3407916

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022616.D
Acq On : 06 Oct 2021 13:00
Operator : SY/MD
Sample : M4051-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

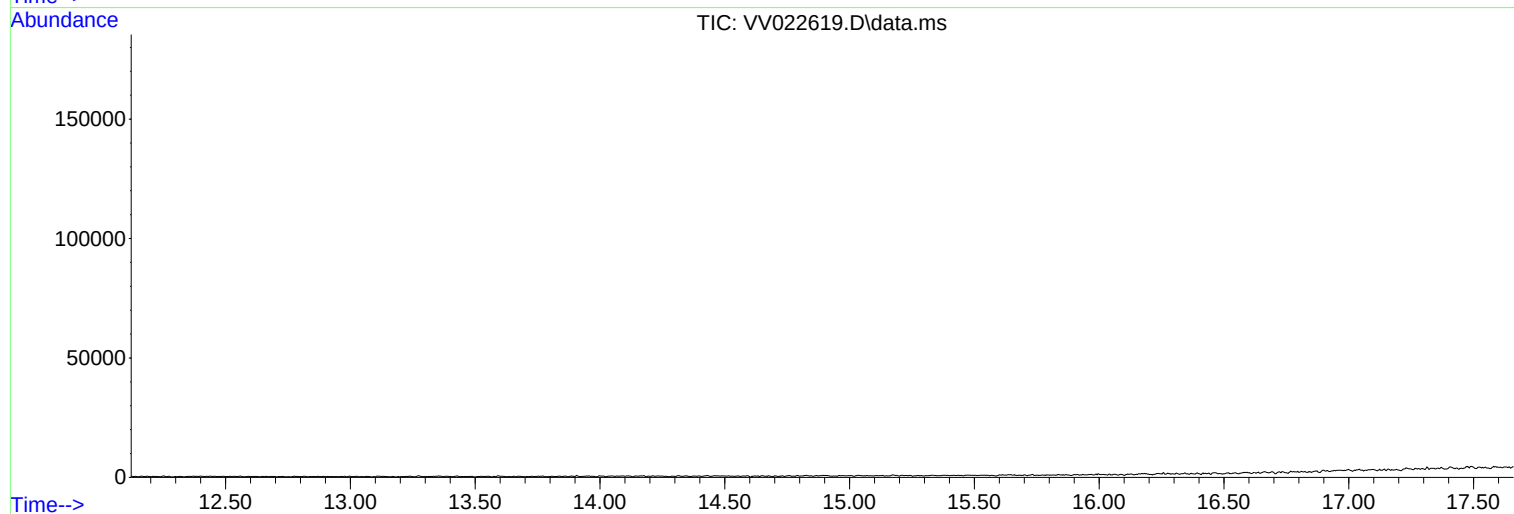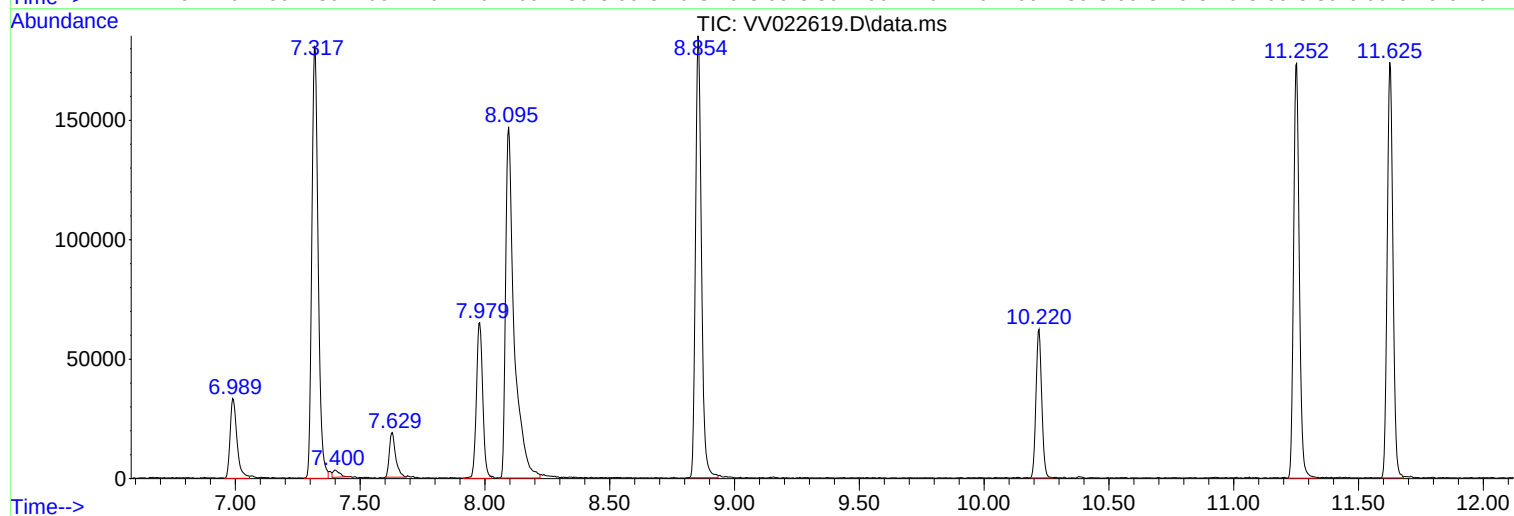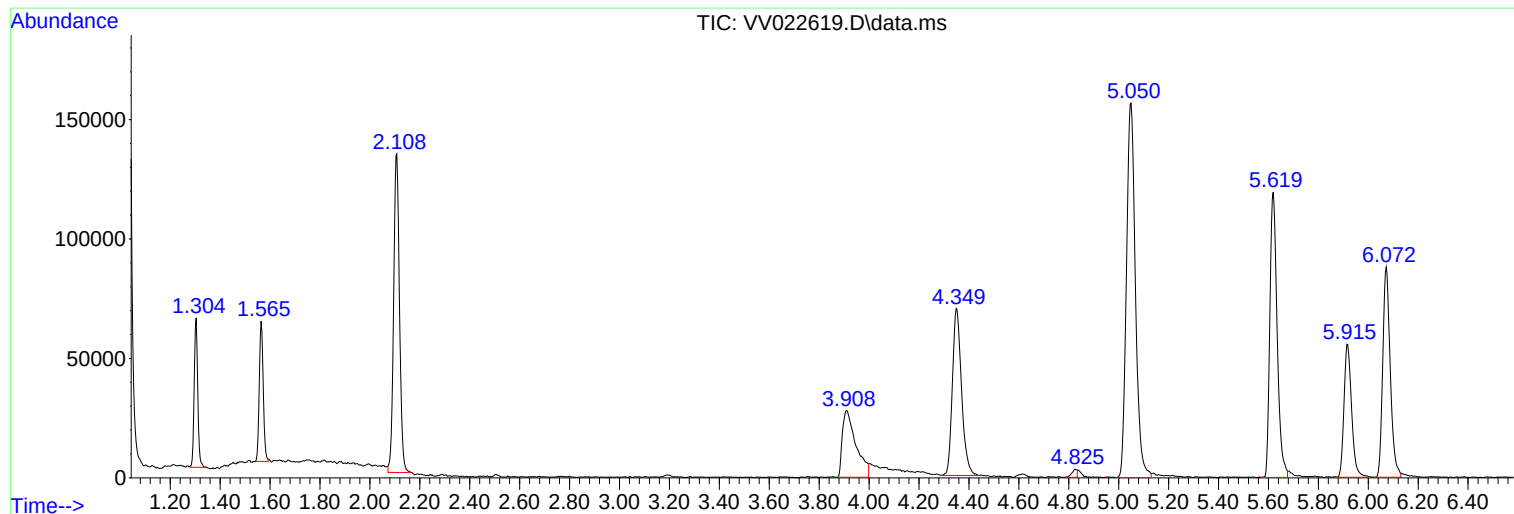

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022616.D
Acq On : 06 Oct 2021 13:00
Operator : SY/MD
Sample : M4051-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022616.D
Acq On : 06 Oct 2021 13:00
Operator : SY/MD
Sample : M4051-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
