

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
 Data File : VV022618.D
 Acq On : 06 Oct 2021 13:49
 Operator : SY/MD
 Sample : M4051-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022621.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	98	rVB	60896	62727	16.75%	1.863%
2	1.568	155	164	175	rBV	55602	64985	17.35%	1.930%
3	2.108	321	332	349	rVB3	127467	205795	54.95%	6.111%
4	3.908	875	892	932	rBV3	61477	225626	60.24%	6.700%
5	4.352	1012	1030	1052	rBV2	65493	166775	44.53%	4.952%
6	4.613	1094	1111	1127	rBV3	5002	11346	3.03%	0.337%
7	5.050	1228	1247	1281	rBV3	150315	374542	100.00%	11.122%
8	5.619	1411	1424	1447	rBV	126361	253284	67.62%	7.521%
9	5.918	1504	1517	1535	rBV2	48654	103304	27.58%	3.068%
10	6.072	1552	1565	1588	rBV	84826	175597	46.88%	5.214%
11	6.989	1840	1850	1868	rBV	32479	59881	15.99%	1.778%
12	7.320	1941	1953	1973	rBV	171850	304229	81.23%	9.034%
13	7.629	2039	2049	2068	rBV2	18066	33686	8.99%	1.000%
14	7.979	2149	2158	2171	rVB2	17067	28607	7.64%	0.849%
15	8.092	2182	2193	2227	rBV2	170306	339545	90.66%	10.083%
16	8.854	2419	2430	2448	rBV	194350	314314	83.92%	9.333%
17	10.220	2844	2855	2872	rBV2	61983	96430	25.75%	2.863%
18	11.249	3164	3175	3195	rBV	180640	283465	75.68%	8.417%
19	11.625	3281	3292	3309	rBV	165755	263486	70.35%	7.824%




Sum of corrected areas: 3367624

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022618.D
Acq On : 06 Oct 2021 13:49
Operator : SY/MD
Sample : M4051-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

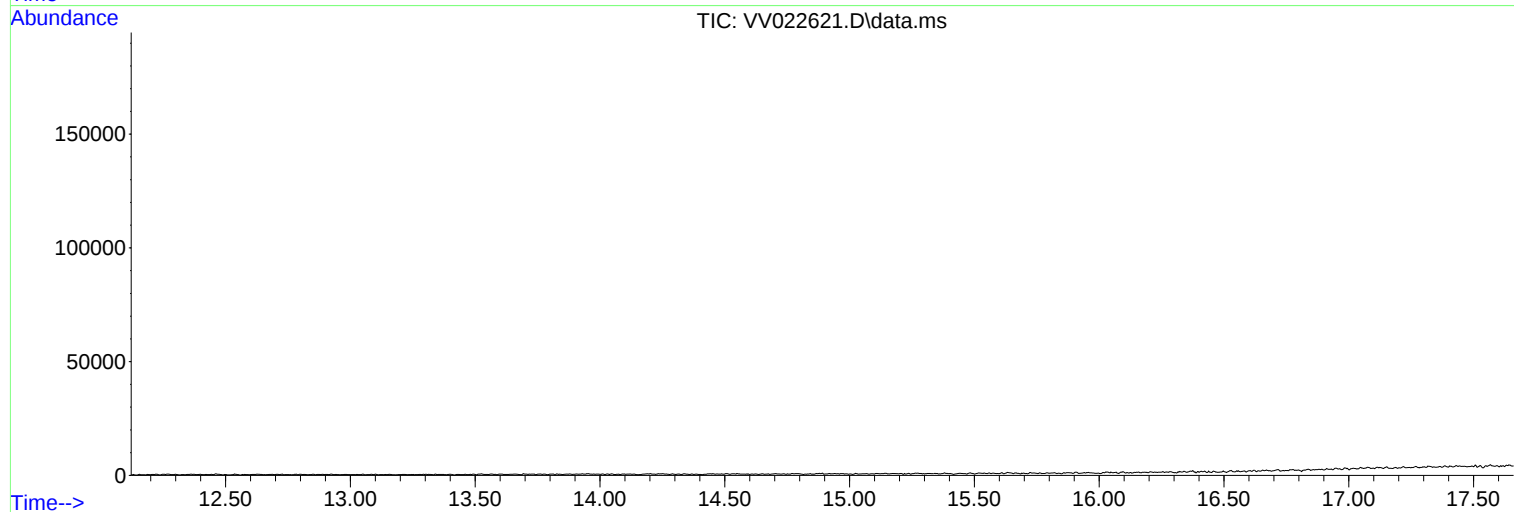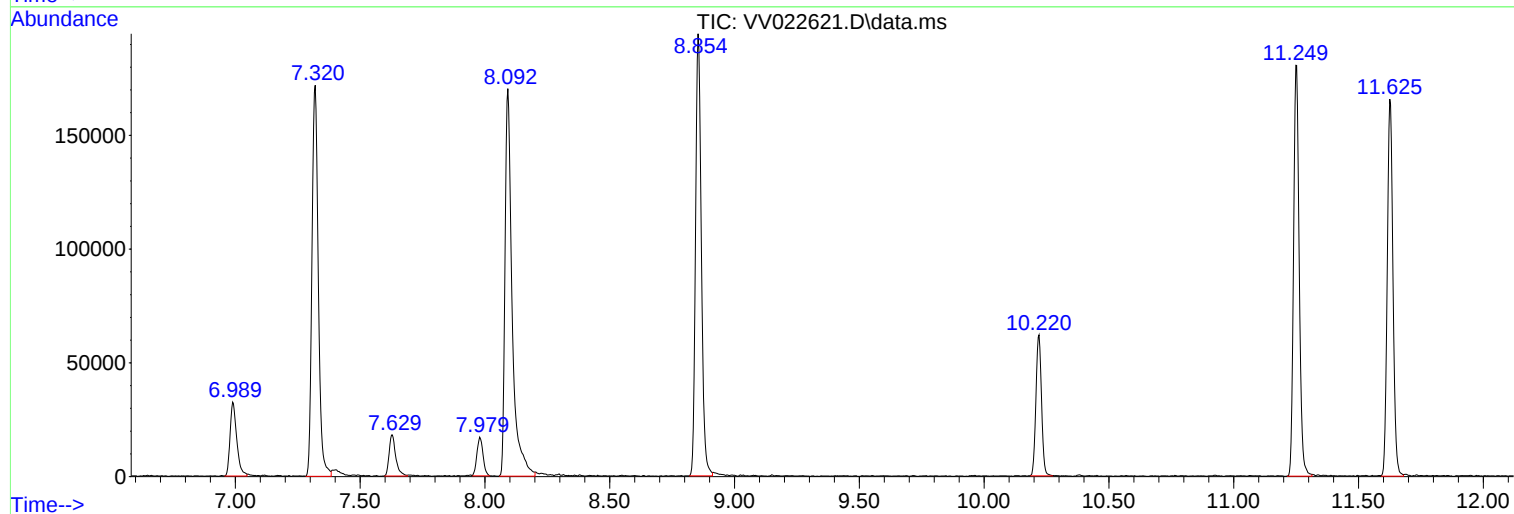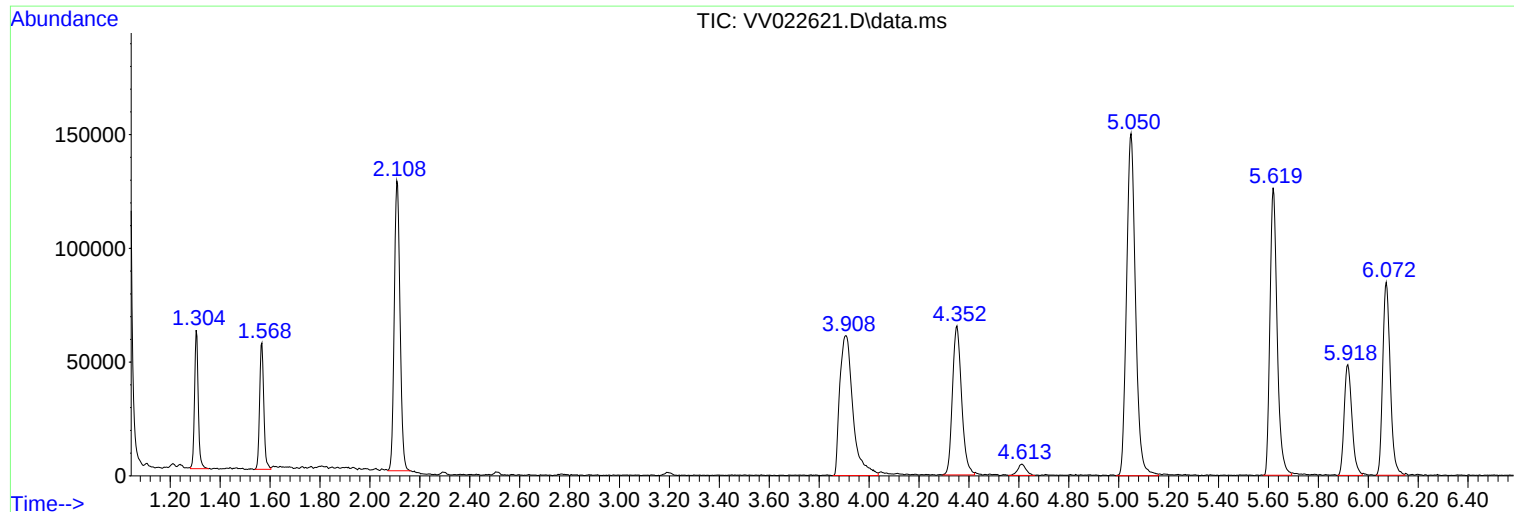

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022618.D
Acq On : 06 Oct 2021 13:49
Operator : SY/MD
Sample : M4051-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022618.D
Acq On : 06 Oct 2021 13:49
Operator : SY/MD
Sample : M4051-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
