

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
 Data File : VV022620.D
 Acq On : 06 Oct 2021 14:37
 Operator : SY/MD
 Sample : M4051-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022620.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	95	rVB	60388	60716	15.63%	1.823%
2	1.568	156	164	172	rBV	56785	65094	16.76%	1.954%
3	2.108	321	332	347	rBV	111588	165155	42.52%	4.958%
4	3.895	878	888	921	rBV	29350	109702	28.24%	3.293%
5	4.349	1014	1029	1057	rVB	66036	176644	45.48%	5.303%
6	4.831	1166	1179	1193	rVB3	3852	9729	2.50%	0.292%
7	5.050	1231	1247	1272	rBV3	156527	388434	100.00%	11.661%
8	5.619	1410	1424	1451	rBV	125877	257215	66.22%	7.722%
9	5.918	1505	1517	1537	rBV5	29820	64162	16.52%	1.926%
10	6.072	1552	1565	1591	rBV	88008	185372	47.72%	5.565%
11	6.989	1840	1850	1867	rBV	33684	63035	16.23%	1.892%
12	7.320	1939	1953	1970	rBV	181001	318610	82.02%	9.565%
13	7.400	1971	1978	1990	rVB3	6036	11256	2.90%	0.338%
14	7.628	2037	2049	2068	rBV	20471	37446	9.64%	1.124%
15	7.979	2148	2158	2172	rVB2	33423	57021	14.68%	1.712%
16	8.091	2182	2193	2236	rBV2	148867	365205	94.02%	10.964%
17	8.853	2419	2430	2452	rBV	195275	322559	83.04%	9.684%
18	10.220	2844	2855	2873	rBV2	62770	102893	26.49%	3.089%
19	11.252	3164	3176	3199	rBV	186425	288807	74.35%	8.670%
20	11.625	3280	3292	3310	rBV	178329	281936	72.58%	8.464%


Sum of corrected areas: 3330991

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022620.D
Acq On : 06 Oct 2021 14:37
Operator : SY/MD
Sample : M4051-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

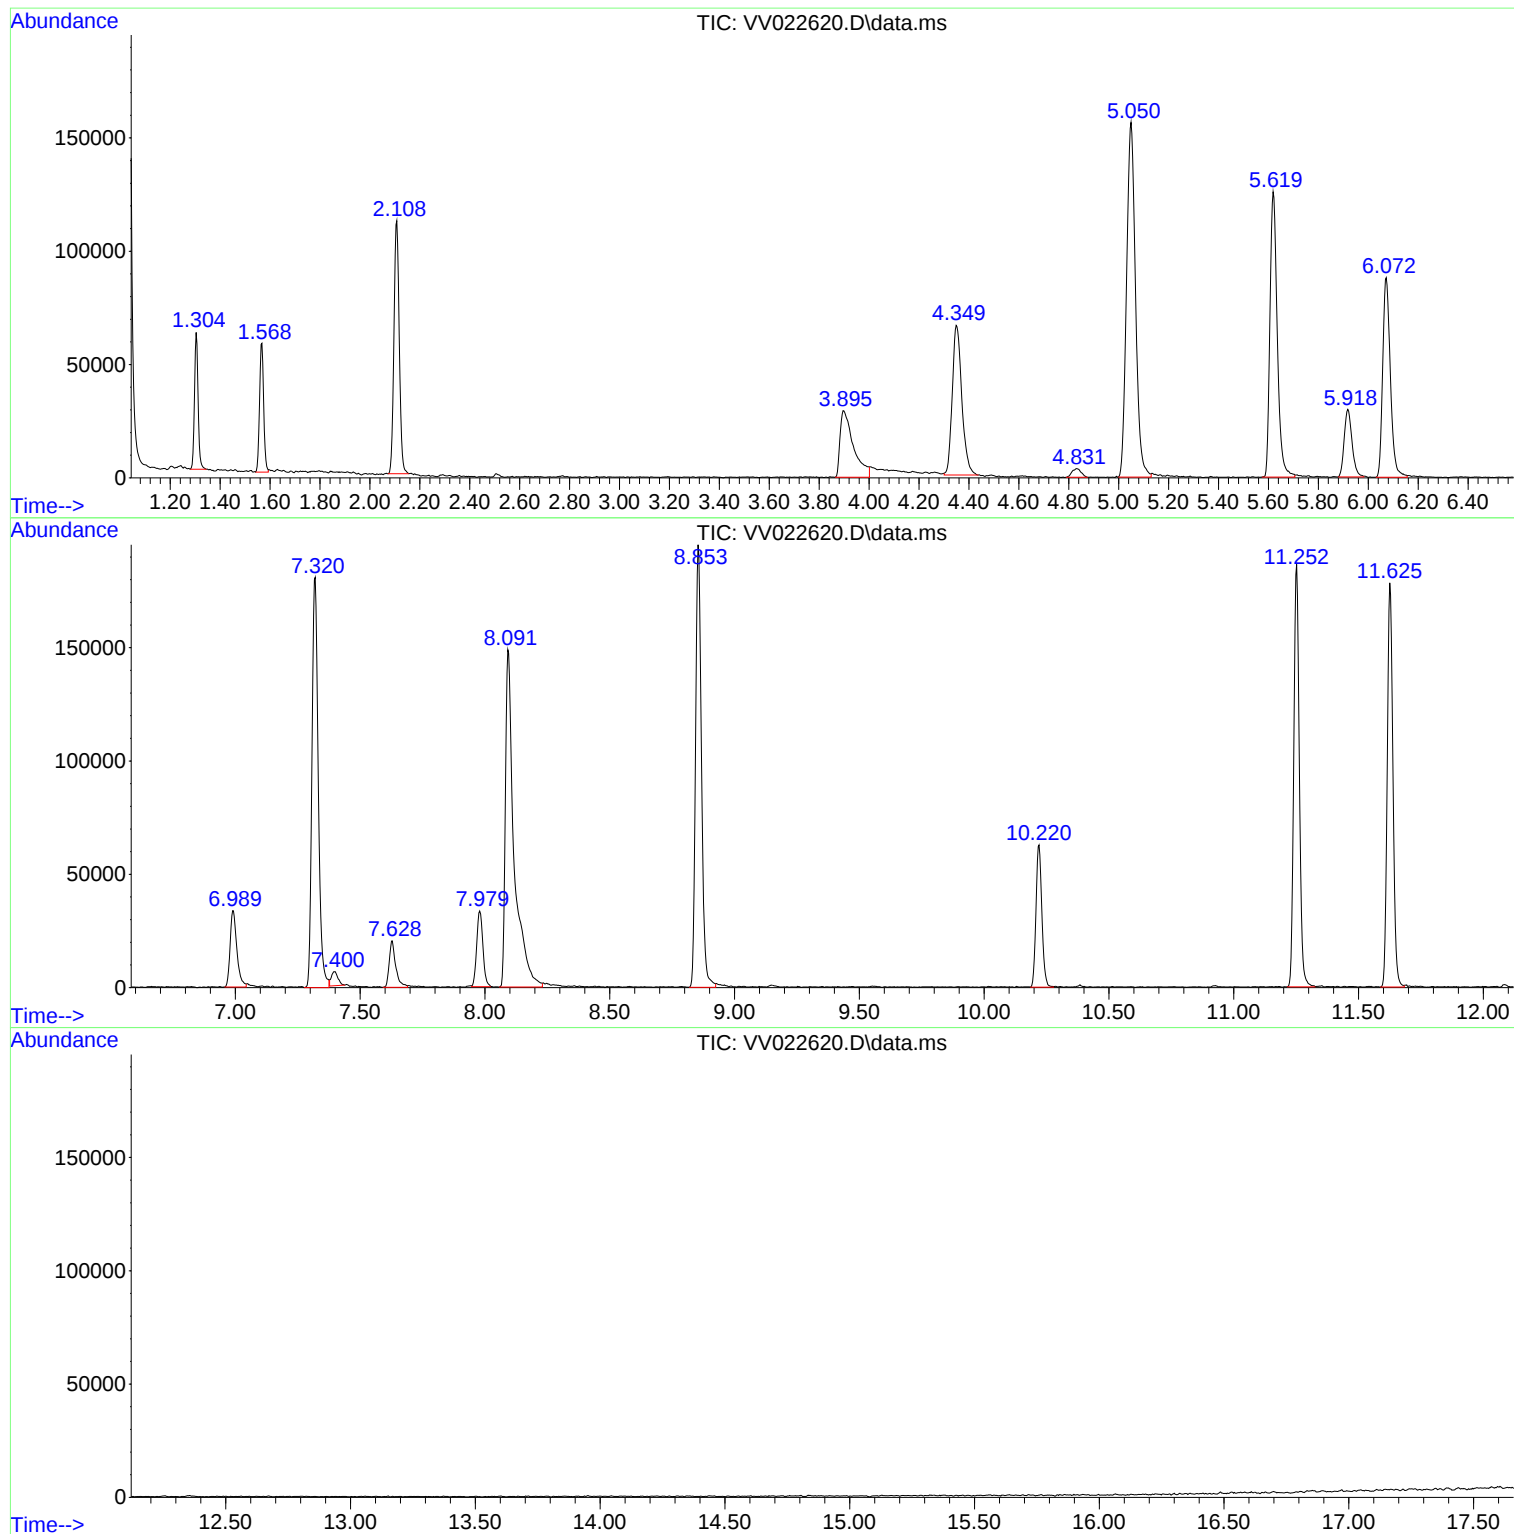

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022620.D
Acq On : 06 Oct 2021 14:37
Operator : SY/MD
Sample : M4051-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022620.D
Acq On : 06 Oct 2021 14:37
Operator : SY/MD
Sample : M4051-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
