

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
 Data File : VV022622.D
 Acq On : 06 Oct 2021 15:25
 Operator : SY/MD
 Sample : M4051-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022622.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rVB	24167	23975	4.98%	0.622%
2	1.564	155	163	172	rBV	35933	42560	8.85%	1.103%
3	1.931	270	277	285	rVB2	5372	7603	1.58%	0.197%
4	2.111	321	333	348	rBV4	152720	248671	51.70%	6.447%
5	3.185	655	667	679	rBV2	4096	8093	1.68%	0.210%
6	3.908	877	892	918	rBV2	190316	480957	100.00%	12.470%
7	4.349	1013	1029	1055	rVB	55003	145579	30.27%	3.775%
8	4.825	1165	1177	1192	rVB7	3418	8769	1.82%	0.227%
9	5.047	1231	1246	1268	rBV2	119059	284828	59.22%	7.385%
10	5.619	1412	1424	1454	rBV	112077	229644	47.75%	5.954%
11	5.912	1503	1515	1542	rBV	192594	384051	79.85%	9.958%
12	6.072	1552	1565	1590	rBV	70432	144726	30.09%	3.752%
13	6.992	1837	1851	1866	rBV	24096	45450	9.45%	1.178%
14	7.317	1940	1952	1970	rBV	111361	198148	41.20%	5.138%
15	7.629	2038	2049	2064	rBV2	14002	25712	5.35%	0.667%
16	7.976	2144	2157	2171	rBV	236331	388914	80.86%	10.084%
17	8.095	2185	2194	2231	rBV2	144717	358166	74.47%	9.286%
18	8.854	2419	2430	2452	rBV	171103	280896	58.40%	7.283%
19	10.217	2844	2854	2871	rBV	56490	90226	18.76%	2.339%
20	11.249	3165	3175	3198	rBV	161371	253438	52.69%	6.571%
21	11.625	3281	3292	3311	rBV	129335	206489	42.93%	5.354%




Sum of corrected areas: 3856895

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022622.D
Acq On : 06 Oct 2021 15:25
Operator : SY/MD
Sample : M4051-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

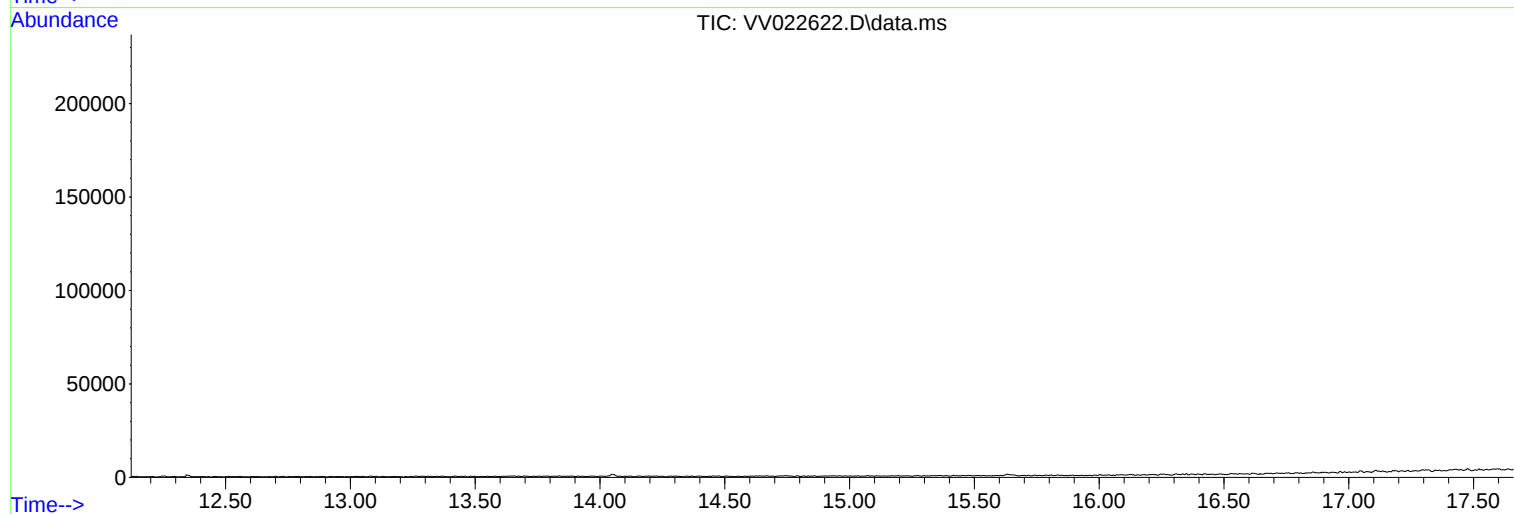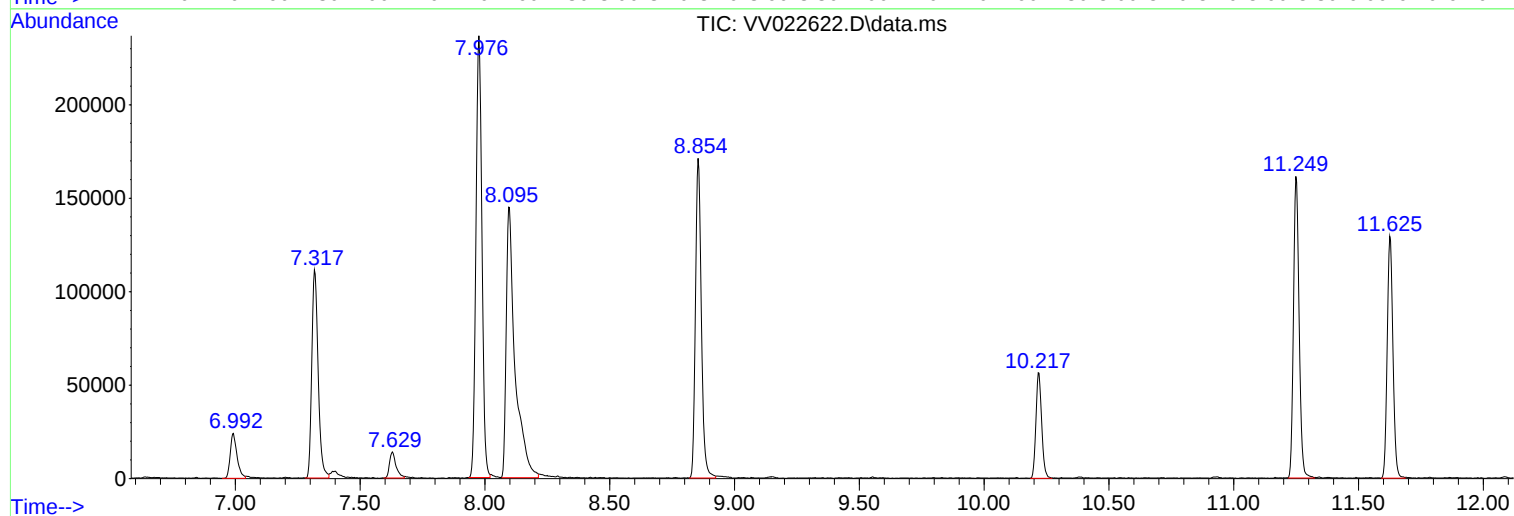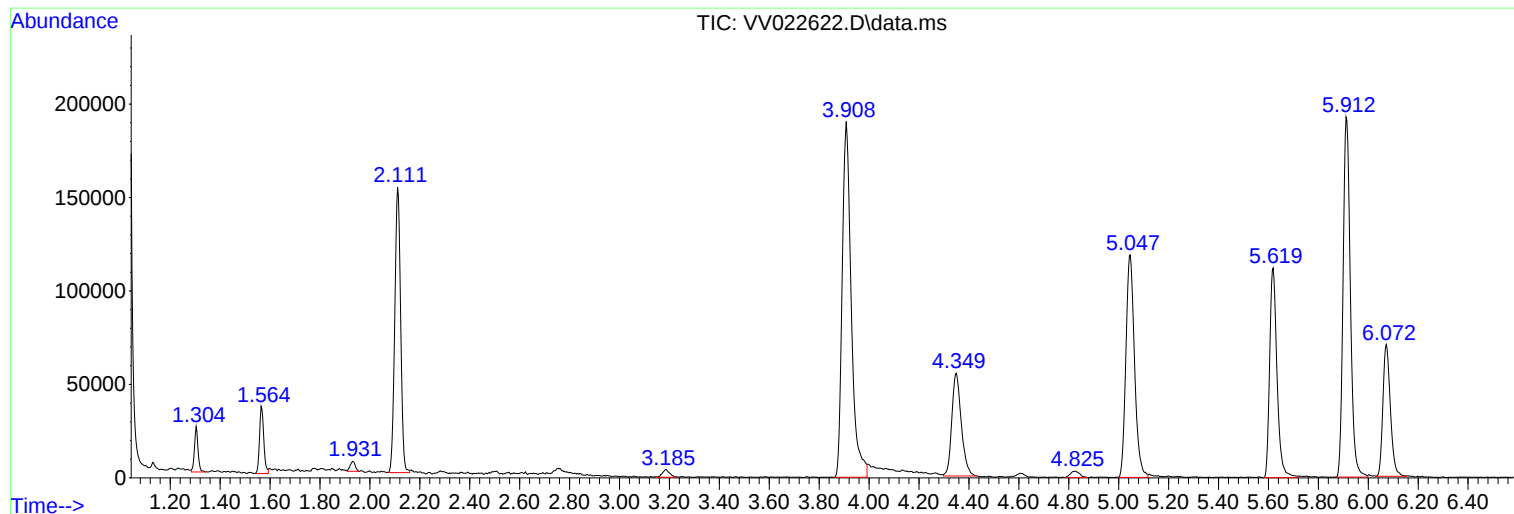

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022622.D
Acq On : 06 Oct 2021 15:25
Operator : SY/MD
Sample : M4051-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022622.D
Acq On : 06 Oct 2021 15:25
Operator : SY/MD
Sample : M4051-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
