

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
 Data File : VV022623.D
 Acq On : 06 Oct 2021 15:49
 Operator : SY/MD
 Sample : M4051-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022623.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	91	rVB	22747	22976	6.28%	0.872%
2	1.565	156	163	171	rBV	36214	40811	11.16%	1.549%
3	2.105	320	331	342	rBV2	54557	80481	22.00%	3.054%
4	3.918	882	895	917	rBV2	32706	114986	31.43%	4.363%
5	4.349	1014	1029	1057	rVB	59019	154153	42.14%	5.849%
6	4.815	1163	1174	1177	rBV6	3476	5181	1.42%	0.197%
7	5.043	1230	1245	1268	rBV3	124885	290394	79.39%	11.019%
8	5.616	1411	1423	1448	rBV	112057	229694	62.79%	8.716%
9	5.915	1502	1516	1530	rBV6	13869	31232	8.54%	1.185%
10	6.072	1552	1565	1588	rBV	75152	152468	41.68%	5.785%
11	6.992	1840	1851	1867	rBV	24600	44433	12.15%	1.686%
12	7.317	1941	1952	1970	rBV	112881	201775	55.16%	7.656%
13	7.394	1970	1976	1986	rVB3	3907	6789	1.86%	0.258%
14	7.629	2038	2049	2059	rBV2	14004	24572	6.72%	0.932%
15	7.976	2141	2157	2170	rVB2	23086	39868	10.90%	1.513%
16	8.098	2185	2195	2231	rBV2	146346	365794	100.00%	13.880%
17	8.854	2417	2430	2453	rBV	171415	284238	77.70%	10.785%
18	10.217	2841	2854	2869	rBV2	56118	92575	25.31%	3.513%
19	11.249	3165	3175	3192	rBV	159888	248335	67.89%	9.423%
20	11.625	3281	3292	3308	rBV	130211	204628	55.94%	7.765%




Sum of corrected areas: 2635383

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022623.D
Acq On : 06 Oct 2021 15:49
Operator : SY/MD
Sample : M4051-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

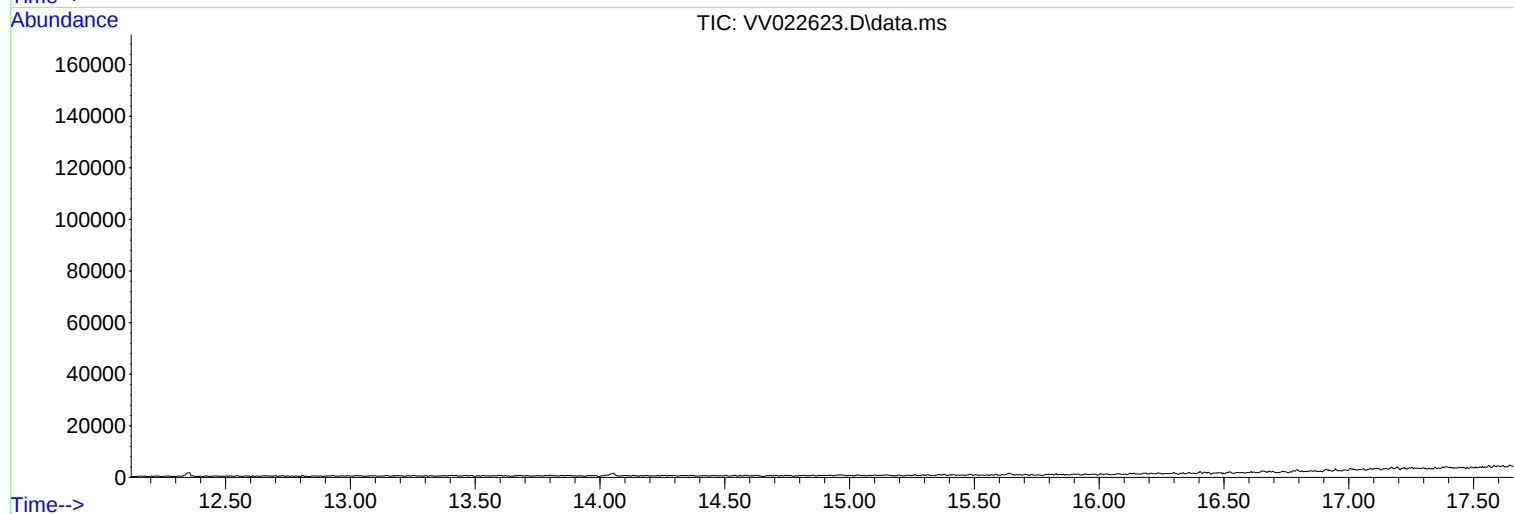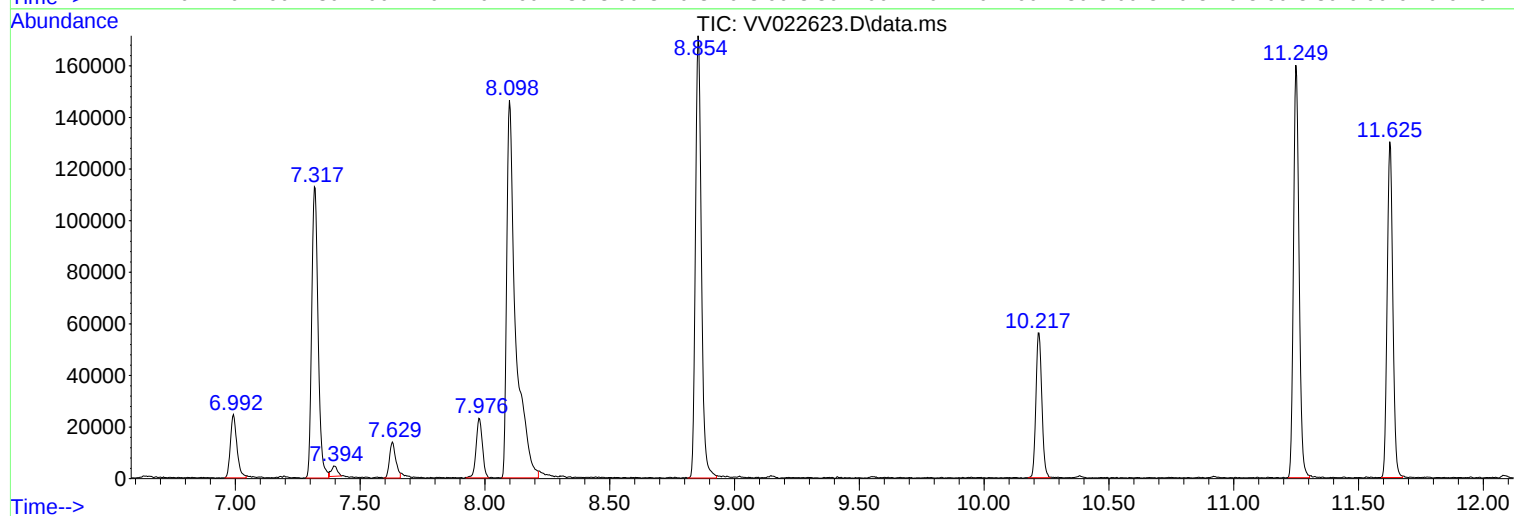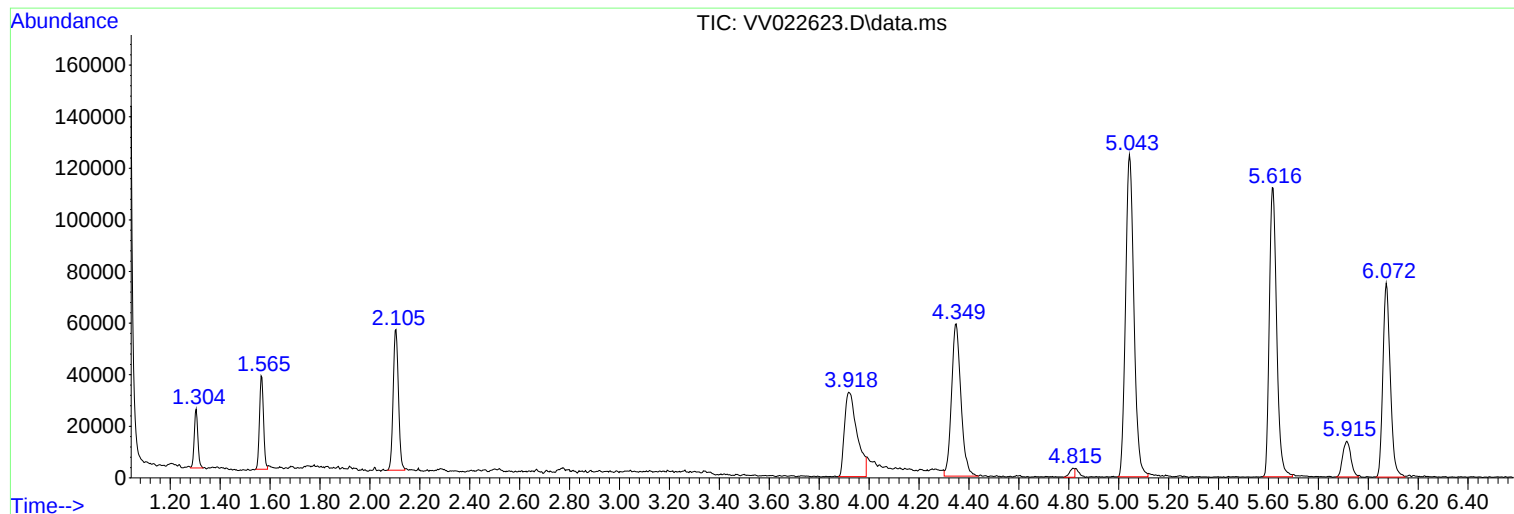

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022623.D
Acq On : 06 Oct 2021 15:49
Operator : SY/MD
Sample : M4051-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022623.D
Acq On : 06 Oct 2021 15:49
Operator : SY/MD
Sample : M4051-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
