

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
 Data File : VV022624.D
 Acq On : 06 Oct 2021 16:13
 Operator : SY/MD
 Sample : M4051-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022624.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	89	rBV	25241	24790	6.66%	0.928%
2	1.564	153	163	177	rBV	41619	49511	13.30%	1.853%
3	2.101	322	330	342	rVB	58021	83966	22.56%	3.142%
4	3.921	880	896	931	rBV	33933	128739	34.59%	4.817%
5	4.346	1015	1028	1052	rVB	61732	155330	41.74%	5.812%
6	5.043	1229	1245	1265	rBV3	128955	304226	81.74%	11.384%
7	5.616	1411	1423	1448	rBV	118155	236065	63.43%	8.833%
8	5.905	1502	1513	1526	rVB8	5283	11435	3.07%	0.428%
9	6.072	1551	1565	1587	rBV	76958	156333	42.00%	5.850%
10	6.992	1841	1851	1868	rBV2	25359	46723	12.55%	1.748%
11	7.316	1938	1952	1969	rBV	120391	211101	56.72%	7.899%
12	7.397	1970	1977	1986	rVB2	3152	6078	1.63%	0.227%
13	7.628	2040	2049	2069	rBV2	14872	26082	7.01%	0.976%
14	7.976	2150	2157	2166	rVB4	4454	7360	1.98%	0.275%
15	8.101	2185	2196	2233	rBV2	147263	372178	100.00%	13.926%
16	8.853	2417	2430	2459	rBV	174017	289901	77.89%	10.848%
17	10.220	2845	2855	2869	rBV	58755	93643	25.16%	3.504%
18	11.249	3165	3175	3200	rBV	161908	256356	68.88%	9.592%
19	11.625	3280	3292	3310	rBV	133107	212646	57.14%	7.957%




Sum of corrected areas: 2672463

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022624.D
Acq On : 06 Oct 2021 16:13
Operator : SY/MD
Sample : M4051-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0AT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

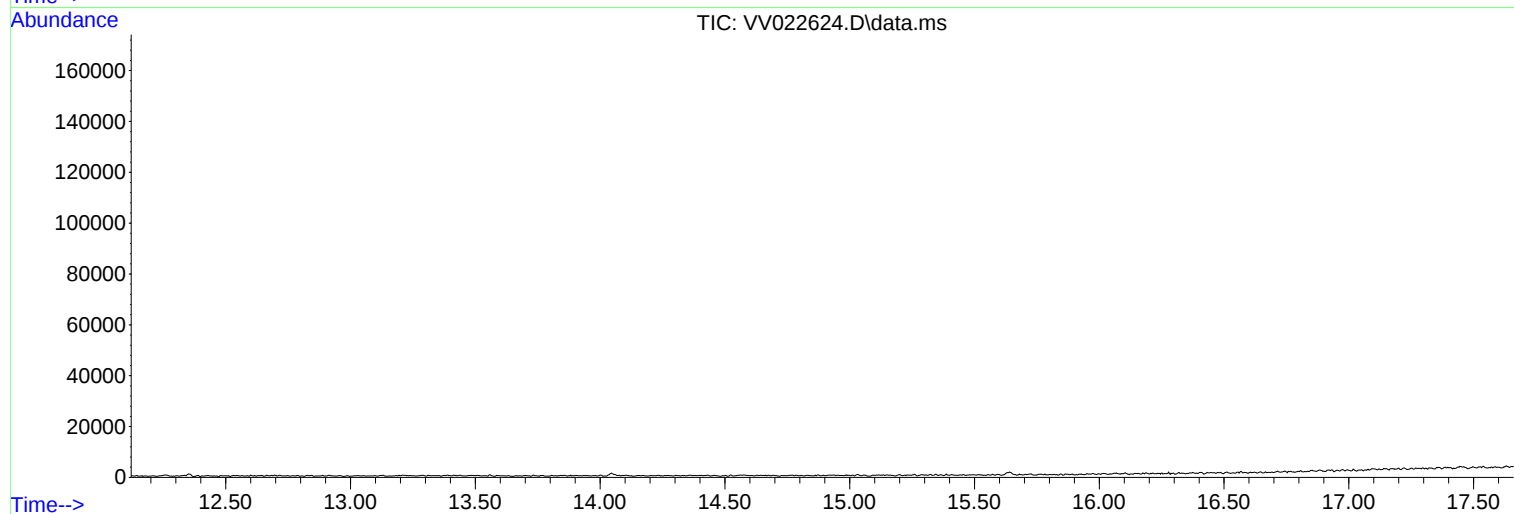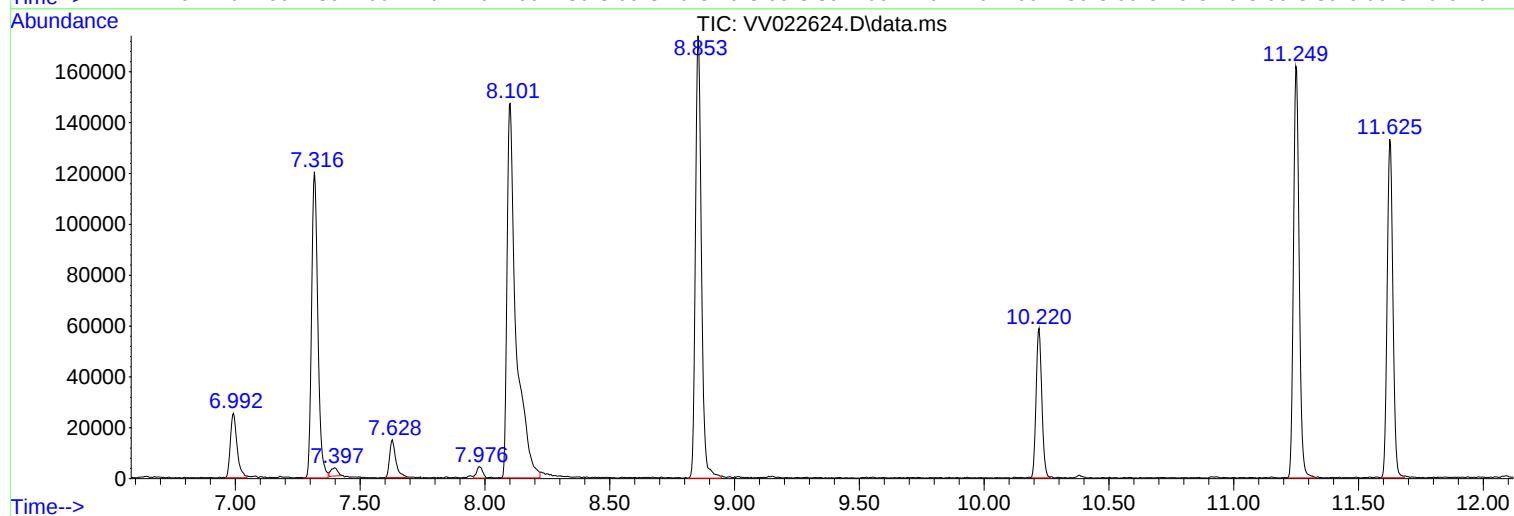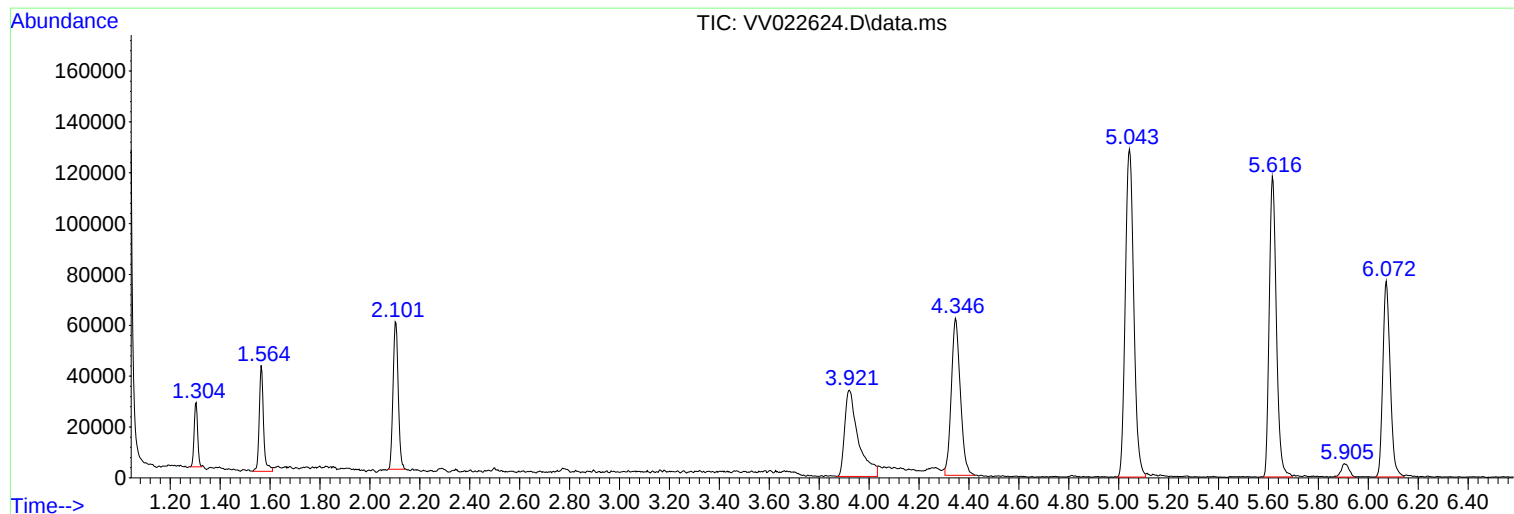

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022624.D
Acq On : 06 Oct 2021 16:13
Operator : SY/MD
Sample : M4051-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022624.D
Acq On : 06 Oct 2021 16:13
Operator : SY/MD
Sample : M4051-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
