

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
 Data File : VV022625.D
 Acq On : 06 Oct 2021 16:37
 Operator : SY/MD
 Sample : M4051-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT3

Integration Parameters: rteint.p

Integrator: RTE

Smoother: ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022625.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.121	17	25	34	rVB	6508	7861	2.21%	0.288%
2	1.294	72	79	91	rVB2	41108	61623	17.30%	2.260%
3	1.565	156	163	176	rBV	37503	44235	12.42%	1.622%
4	2.108	322	332	346	rBV	58772	85999	24.15%	3.153%
5	2.294	379	390	400	rBV	21171	31668	8.89%	1.161%
6	3.886	874	885	922	rBV	49066	151585	42.57%	5.558%
7	4.349	1011	1029	1052	rBV2	57552	149580	42.00%	5.485%
8	5.050	1230	1247	1273	rBV3	114831	294084	82.58%	10.783%
9	5.619	1411	1424	1446	rBV	113641	234652	65.89%	8.604%
10	5.908	1504	1514	1529	rVB5	7690	16400	4.61%	0.601%
11	6.072	1551	1565	1585	rBV2	73617	150774	42.34%	5.529%
12	6.989	1841	1850	1868	rBV3	24430	45597	12.80%	1.672%
13	7.320	1939	1953	1971	rBV	116313	205586	57.73%	7.538%
14	7.629	2038	2049	2061	rBV	14716	25331	7.11%	0.929%
15	8.092	2183	2193	2228	rBV2	167969	356123	100.00%	13.058%
16	8.854	2419	2430	2451	rBV	176983	293358	82.38%	10.757%
17	10.217	2842	2854	2865	rBV2	51733	82504	23.17%	3.025%
18	11.249	3165	3175	3194	rBV	164253	261768	73.50%	9.598%
19	11.625	3281	3292	3311	rBV	132405	212346	59.63%	7.786%
20	16.561	4816	4827	4842	rBV2	9927	16139	4.53%	0.592%




Sum of corrected areas: 2727213

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022625.D
Acq On : 06 Oct 2021 16:37
Operator : SY/MD
Sample : M4051-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

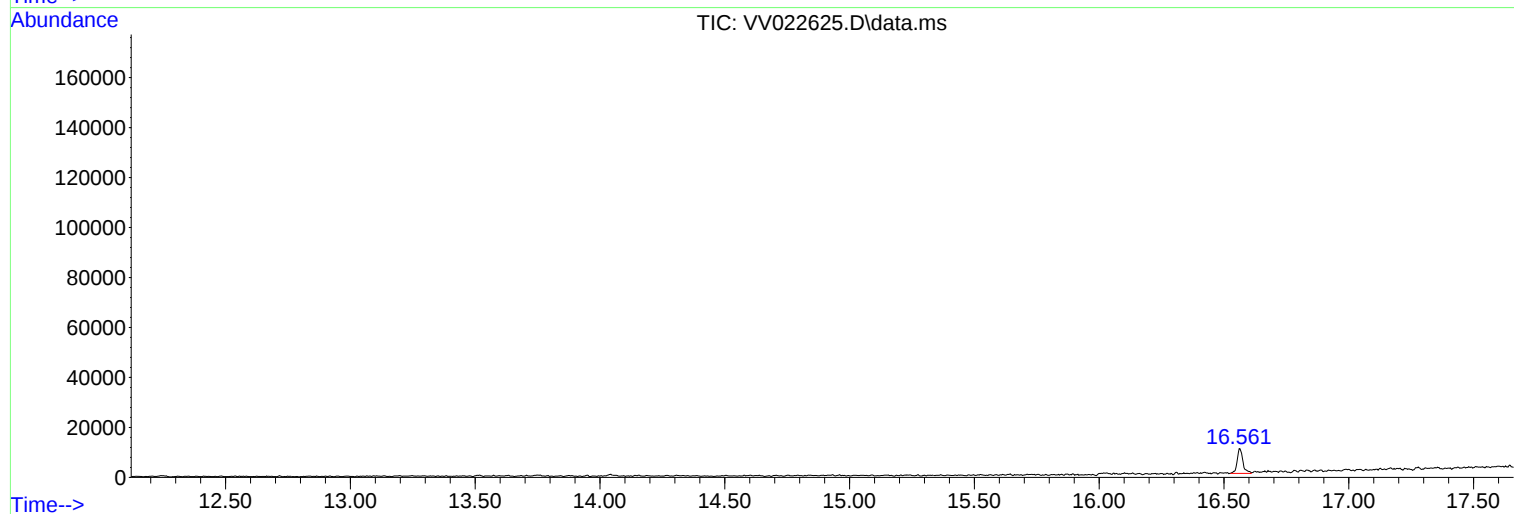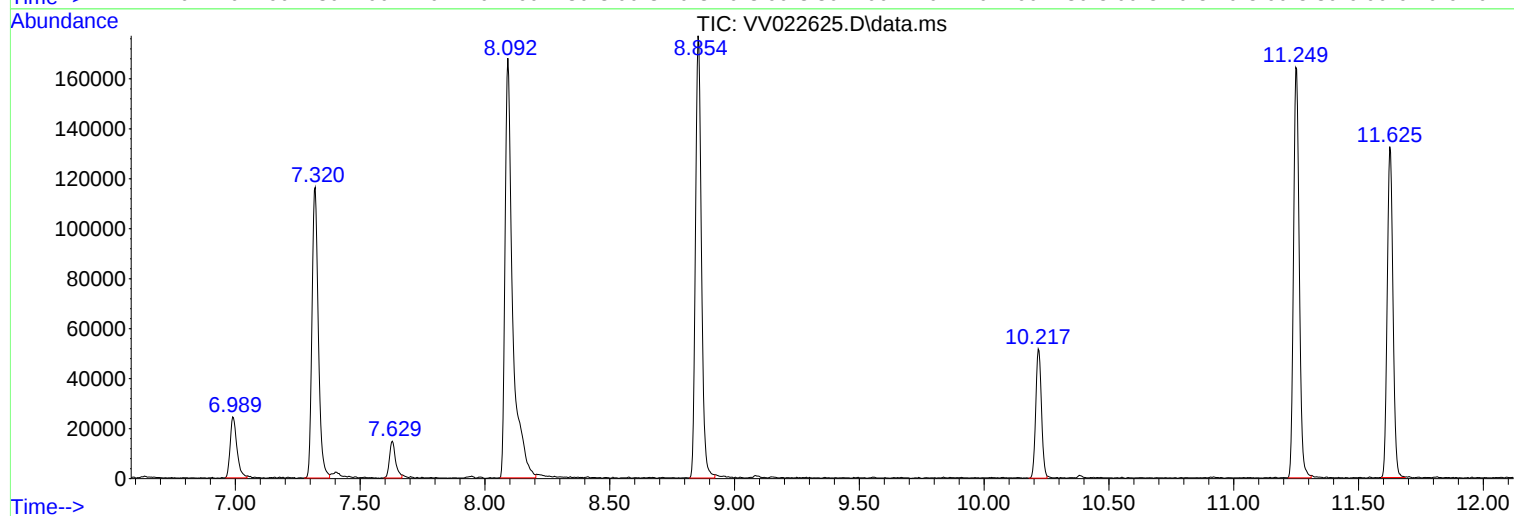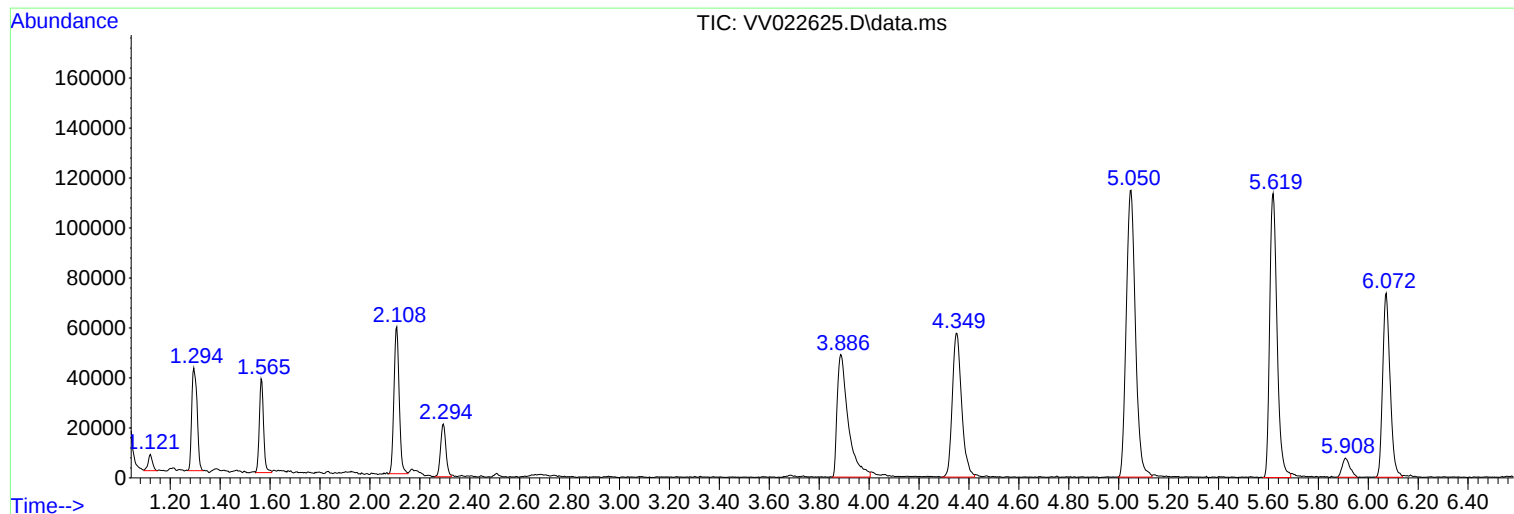

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022625.D
Acq On : 06 Oct 2021 16:37
Operator : SY/MD
Sample : M4051-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022625.D
Acq On : 06 Oct 2021 16:37
Operator : SY/MD
Sample : M4051-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
