

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
 Data File : VV022630.D
 Acq On : 06 Oct 2021 18:37
 Operator : SY/MD
 Sample : M4051-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT9

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022630.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	91	rVB	21694	22534	5.83%	0.774%
2	1.565	155	163	173	rBV	35191	39970	10.34%	1.373%
3	2.108	322	332	346	rBV3	74158	126176	32.63%	4.334%
4	3.896	877	888	926	rBV2	48064	177959	46.02%	6.113%
5	4.352	1013	1030	1061	rBV4	50640	145991	37.75%	5.015%
6	5.047	1231	1246	1276	rBV2	107812	275345	71.20%	9.458%
7	5.619	1411	1424	1447	rBV	108903	222418	57.52%	7.640%
8	5.918	1503	1517	1540	rBV3	84019	179034	46.30%	6.150%
9	6.072	1552	1565	1584	rBV	68219	142367	36.81%	4.890%
10	6.992	1841	1851	1867	rBV2	22309	42861	11.08%	1.472%
11	7.320	1942	1953	1970	rBV	108283	191640	49.56%	6.583%
12	7.629	2040	2049	2064	rBV2	13621	24820	6.42%	0.853%
13	7.979	2147	2158	2176	rVB	61930	102875	26.60%	3.534%
14	8.092	2182	2193	2228	rBV2	192875	386712	100.00%	13.283%
15	8.854	2419	2430	2450	rBV	169659	280830	72.62%	9.646%
16	10.220	2841	2855	2872	rBV2	58756	92922	24.03%	3.192%
17	11.249	3165	3175	3195	rBV	160282	248985	64.39%	8.552%
18	11.628	3281	3293	3310	rBV	124065	201089	52.00%	6.907%
19	16.564	4821	4828	4836	rVB2	5356	6773	1.75%	0.233%




Sum of corrected areas: 2911301

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022630.D
Acq On : 06 Oct 2021 18:37
Operator : SY/MD
Sample : M4051-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

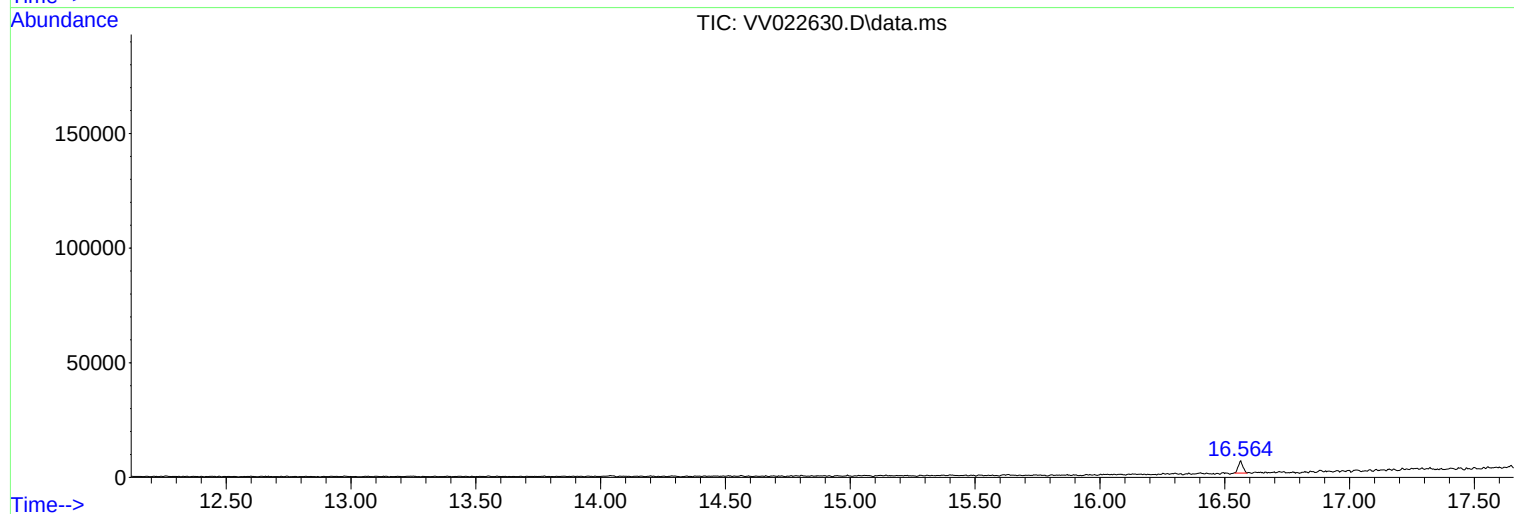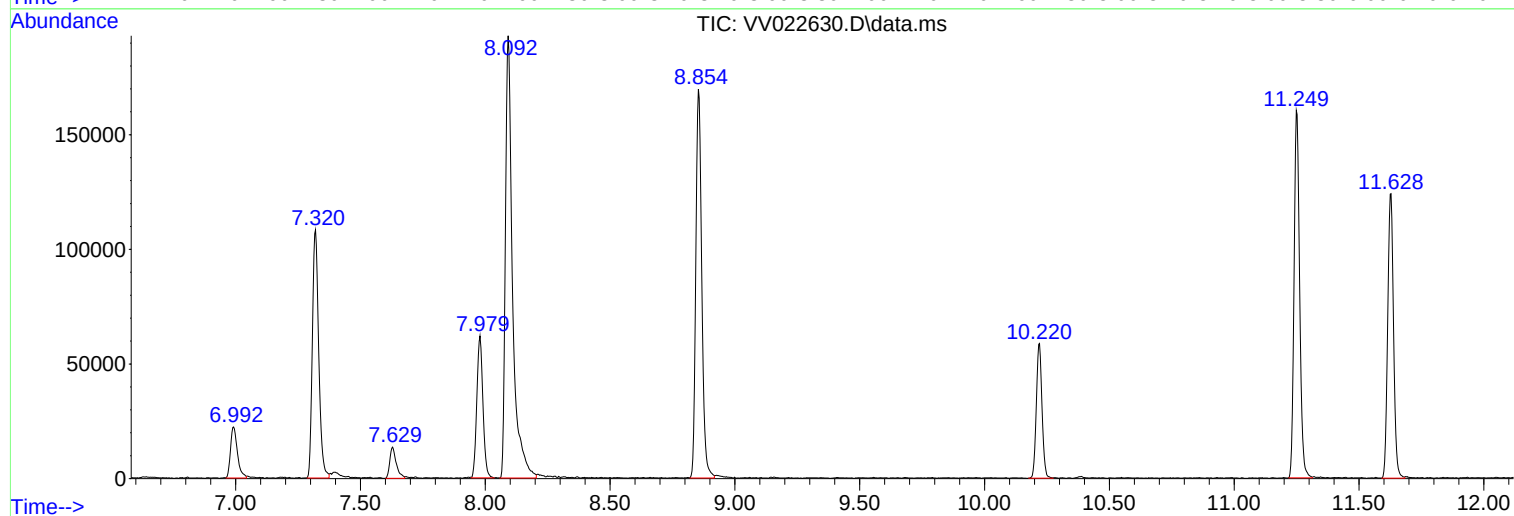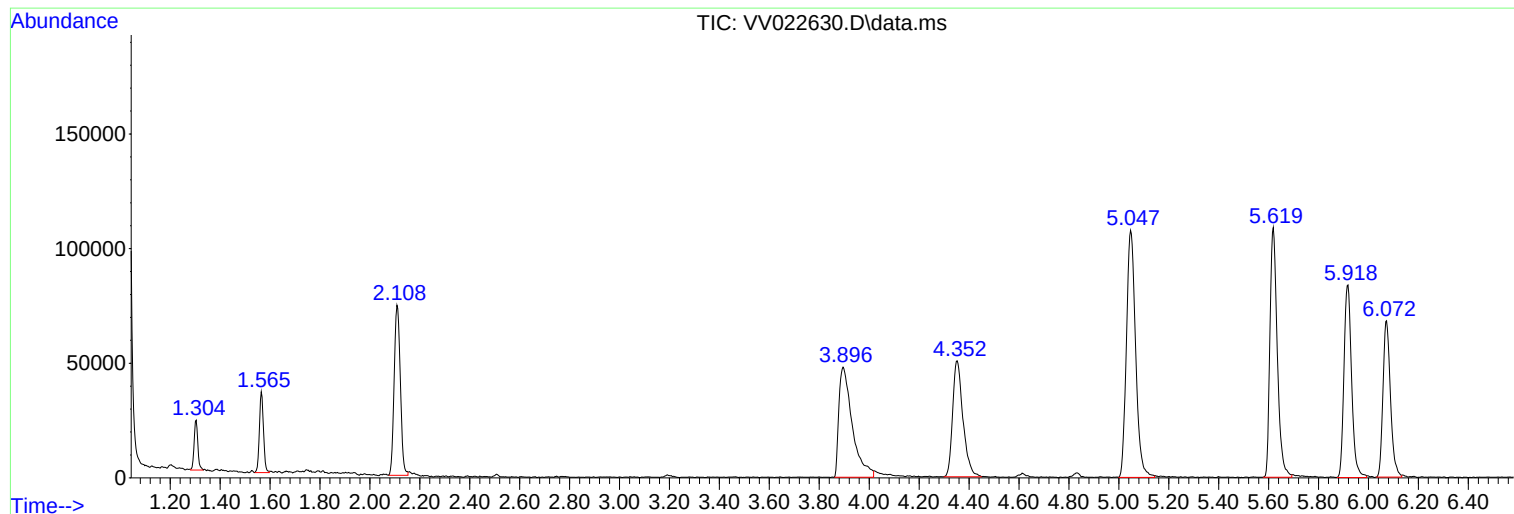

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022630.D
Acq On : 06 Oct 2021 18:37
Operator : SY/MD
Sample : M4051-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022630.D
Acq On : 06 Oct 2021 18:37
Operator : SY/MD
Sample : M4051-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
