

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
 Data File : VV022631.D
 Acq On : 06 Oct 2021 19:02
 Operator : SY/MD
 Sample : M4050-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7B7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022631.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	15	20	25	rBV	19954	16441	4.95%	0.652%
2	1.175	37	42	46	rBV2	5397	4908	1.48%	0.195%
3	1.301	73	81	95	rVB2	28332	34554	10.40%	1.371%
4	1.565	153	163	173	rBV	32628	38686	11.65%	1.535%
5	2.105	317	331	342	rBV	52137	77726	23.40%	3.084%
6	2.169	345	351	360	rVB2	3237	5751	1.73%	0.228%
7	2.294	379	390	402	rVB2	4010	6360	1.91%	0.252%
8	3.880	873	883	928	rBV	47763	142305	42.84%	5.646%
9	4.349	1014	1029	1050	rBV	48918	125780	37.87%	4.990%
10	5.047	1228	1246	1277	rBV4	103153	264090	79.51%	10.478%
11	5.619	1412	1424	1444	rBV2	106203	219321	66.03%	8.702%
12	5.912	1503	1515	1529	rBV8	4421	9614	2.89%	0.381%
13	6.072	1551	1565	1583	rBV2	66174	138279	41.63%	5.486%
14	6.992	1839	1851	1871	rBV	22083	41762	12.57%	1.657%
15	7.320	1941	1953	1970	rBV	105007	185678	55.90%	7.367%
16	7.629	2040	2049	2064	rBV	13213	22901	6.89%	0.909%
17	8.088	2183	2192	2229	rBV2	166045	332140	100.00%	13.178%
18	8.854	2419	2430	2450	rBV	166781	274593	82.67%	10.894%
19	9.815	2723	2729	2740	rBV4	2486	3693	1.11%	0.147%
20	10.217	2844	2854	2872	rVB2	53326	83679	25.19%	3.320%
21	11.153	3138	3145	3154	rVB4	5310	7548	2.27%	0.299%
22	11.249	3165	3175	3190	rBV	161656	252392	75.99%	10.014%
23	11.535	3256	3264	3274	rBV5	2980	4896	1.47%	0.194%
24	11.625	3281	3292	3315	rVB	123424	197680	59.52%	7.843%
25	12.345	3507	3516	3526	rBV4	11090	16805	5.06%	0.667%
26	13.606	3899	3908	3915	rBV3	2492	3663	1.10%	0.145%
27	16.564	4820	4828	4836	rBV3	3786	5795	1.74%	0.230%
28	17.101	4988	4995	5001	rVB3	2887	3438	1.04%	0.136%




Sum of corrected areas: 2520478

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022631.D
Acq On : 06 Oct 2021 19:02
Operator : SY/MD
Sample : M4050-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7B7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

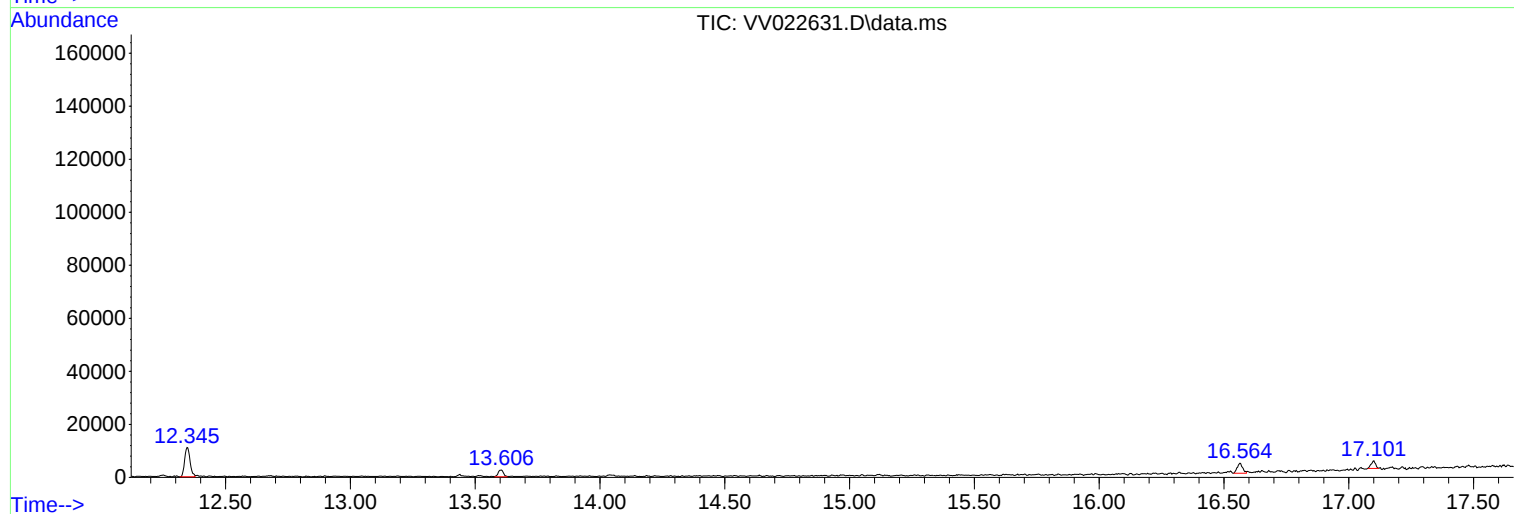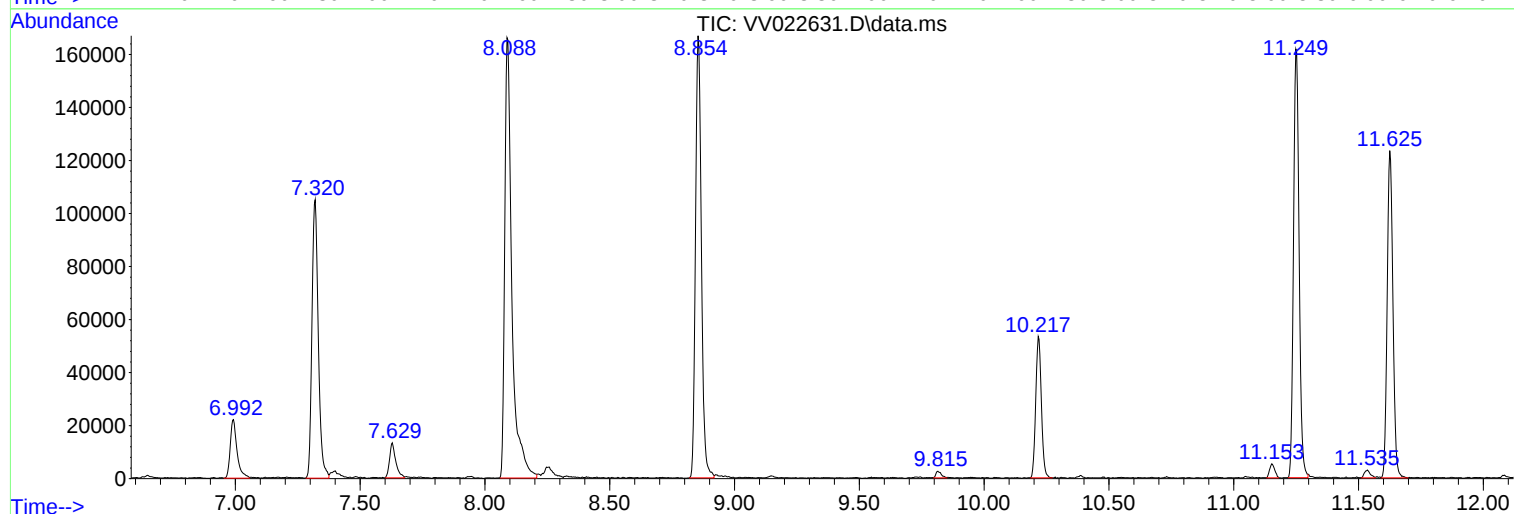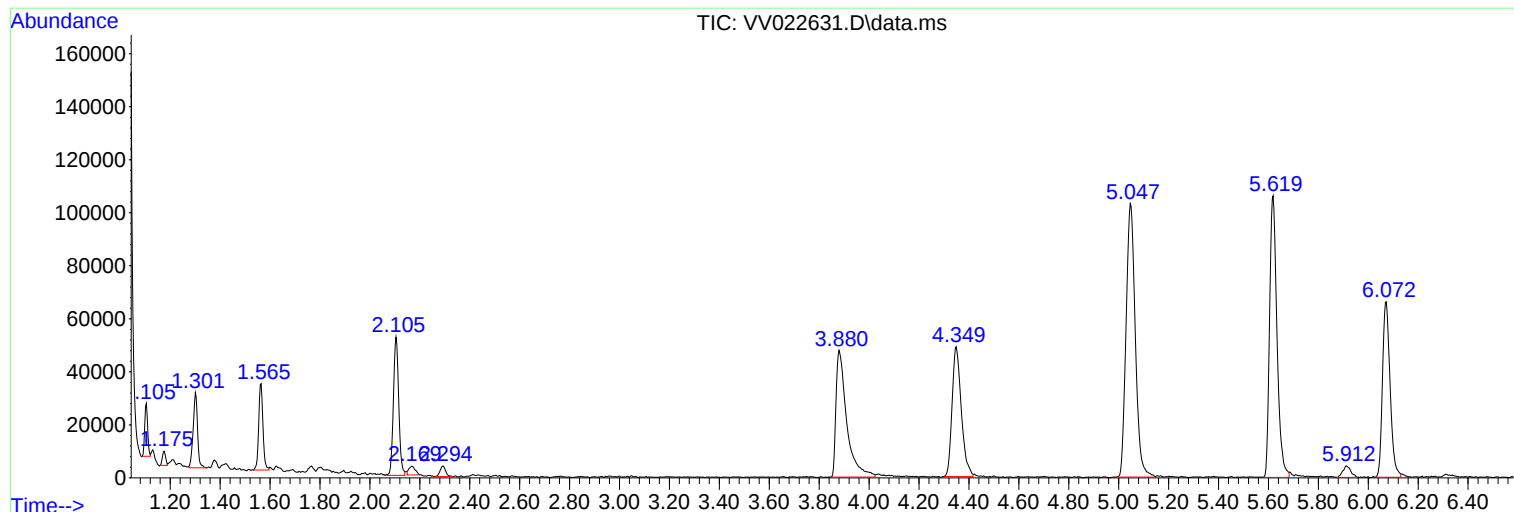

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022631.D
Acq On : 06 Oct 2021 19:02
Operator : SY/MD
Sample : M4050-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7B7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022631.D
Acq On : 06 Oct 2021 19:02
Operator : SY/MD
Sample : M4050-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7B7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
