

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
 Data File : VV022632.D
 Acq On : 06 Oct 2021 19:26
 Operator : SY/MD
 Sample : M4050-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7B8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022632.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.130	25	28	36	rVB	4759	4854	1.42%	0.193%
2	1.304	74	82	92	rVB	23859	26786	7.84%	1.064%
3	1.565	156	163	175	rVB2	35779	43854	12.83%	1.741%
4	2.105	321	331	343	rBV	52357	77529	22.68%	3.079%
5	3.883	872	884	915	rBV	49657	146359	42.81%	5.812%
6	4.349	1014	1029	1055	rBV2	51957	133051	38.92%	5.284%
7	5.047	1231	1246	1272	rBV2	108984	276162	80.79%	10.967%
8	5.619	1412	1424	1444	rBV	107350	220592	64.53%	8.760%
9	5.915	1505	1516	1530	rBV10	4765	10651	3.12%	0.423%
10	6.072	1551	1565	1591	rBV2	69216	143888	42.09%	5.714%
11	6.992	1840	1851	1870	rBV	22813	43138	12.62%	1.713%
12	7.320	1942	1953	1969	rBV	108710	193347	56.56%	7.678%
13	7.629	2037	2049	2064	rBV3	13579	25649	7.50%	1.019%
14	8.092	2182	2193	2228	rBV2	173579	341845	100.00%	13.575%
15	8.854	2420	2430	2452	rBV	168393	277005	81.03%	11.000%
16	10.217	2844	2854	2872	rBV	56161	88078	25.77%	3.498%
17	11.252	3164	3176	3193	rBV	156928	246829	72.20%	9.802%
18	11.532	3255	3263	3274	rBV2	2750	4520	1.32%	0.179%
19	11.625	3281	3292	3315	rVB	130325	205712	60.18%	8.169%
20	12.352	3510	3518	3528	rBV4	2873	4068	1.19%	0.162%
21	16.561	4820	4827	4837	rBV6	2838	4295	1.26%	0.171%




Sum of corrected areas: 2518212

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022632.D
Acq On : 06 Oct 2021 19:26
Operator : SY/MD
Sample : M4050-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
GB7B8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

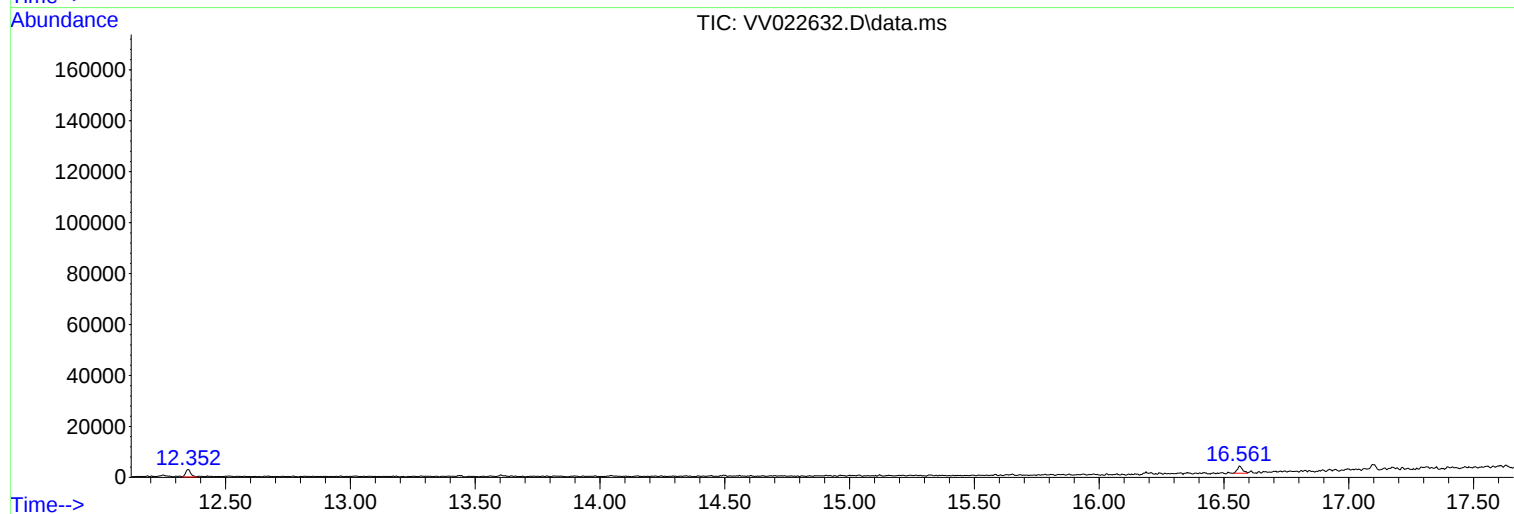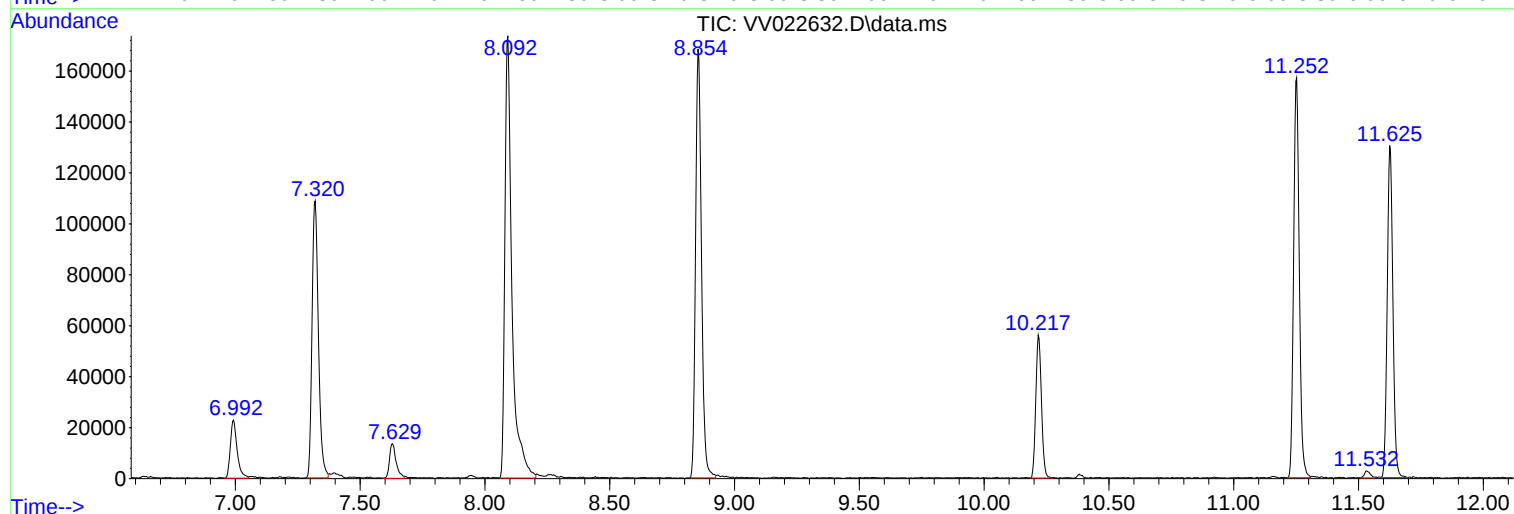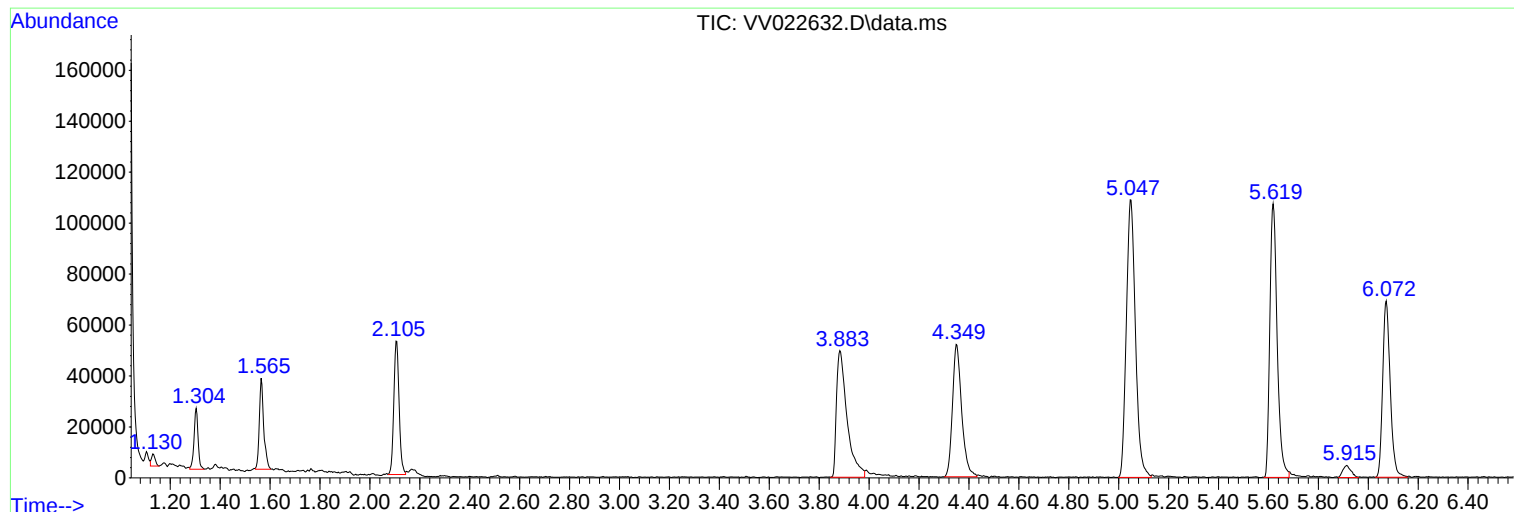

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022632.D
Acq On : 06 Oct 2021 19:26
Operator : SY/MD
Sample : M4050-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7B8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022632.D
Acq On : 06 Oct 2021 19:26
Operator : SY/MD
Sample : M4050-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7B8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
