

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
 Data File : VV022645.D
 Acq On : 07 Oct 2021 01:27
 Operator : SY/MD
 Sample : M4050-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7C7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022645.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	23	29	40	rVB	6447	6801	1.89%	0.249%
2	1.301	71	81	96	rBV2	25832	37468	10.42%	1.374%
3	1.564	156	163	174	rBV	34261	38623	10.74%	1.416%
4	2.105	320	331	342	rBV	53755	77580	21.57%	2.845%
5	2.188	348	357	368	rBV2	3321	8328	2.32%	0.305%
6	3.902	879	890	918	rBV2	36093	136362	37.91%	5.001%
7	4.349	1014	1029	1054	rBV	53154	133929	37.23%	4.912%
8	5.050	1232	1247	1271	rBV3	111371	284120	78.99%	10.419%
9	5.619	1412	1424	1455	rBV	115021	233644	64.95%	8.568%
10	5.908	1504	1514	1529	rBV6	7670	17481	4.86%	0.641%
11	6.072	1553	1565	1585	rBV	71158	146927	40.85%	5.388%
12	6.587	1713	1725	1734	rBV6	2814	6197	1.72%	0.227%
13	6.992	1841	1851	1870	rBV2	23028	44098	12.26%	1.617%
14	7.320	1942	1953	1968	rBV	113717	198810	55.27%	7.291%
15	7.397	1969	1977	1994	rVB	12774	23824	6.62%	0.874%
16	7.629	2038	2049	2066	rBV3	13659	25650	7.13%	0.941%
17	7.979	2150	2158	2171	rVB2	12431	21161	5.88%	0.776%
18	8.092	2182	2193	2226	rBV2	161162	359713	100.00%	13.192%
19	8.854	2420	2430	2457	rBV	178325	291418	81.01%	10.687%
20	8.966	2459	2465	2473	rVB6	3325	4918	1.37%	0.180%
21	9.021	2474	2482	2493	rBV3	3474	5086	1.41%	0.187%
22	9.143	2511	2520	2536	rVB2	14705	25256	7.02%	0.926%
23	9.551	2637	2647	2663	rBV5	8596	18531	5.15%	0.680%
24	10.217	2844	2854	2871	rVB	50887	80223	22.30%	2.942%
25	10.921	3061	3073	3084	rBV5	2666	3951	1.10%	0.145%
26	11.252	3164	3176	3196	rBV	171969	269034	74.79%	9.866%
27	11.532	3254	3263	3277	rBV2	6712	10588	2.94%	0.388%
28	11.625	3282	3292	3308	rBV	134119	217115	60.36%	7.962%




Sum of corrected areas: 2726836

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022645.D
Acq On : 07 Oct 2021 01:27
Operator : SY/MD
Sample : M4050-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7C7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

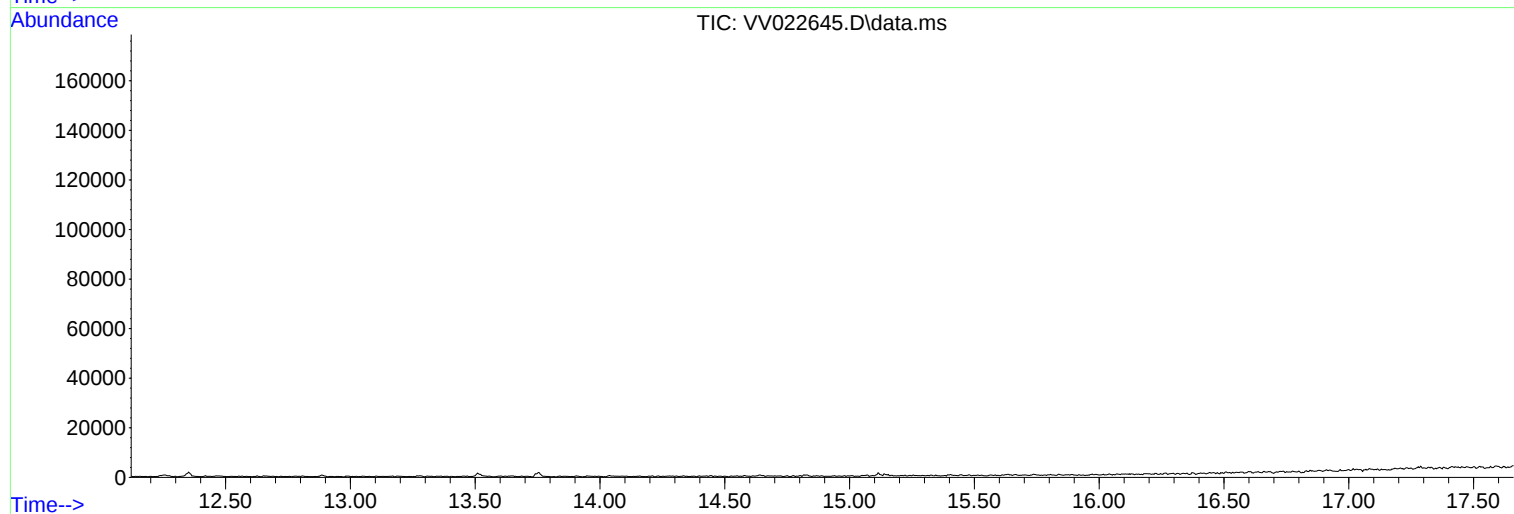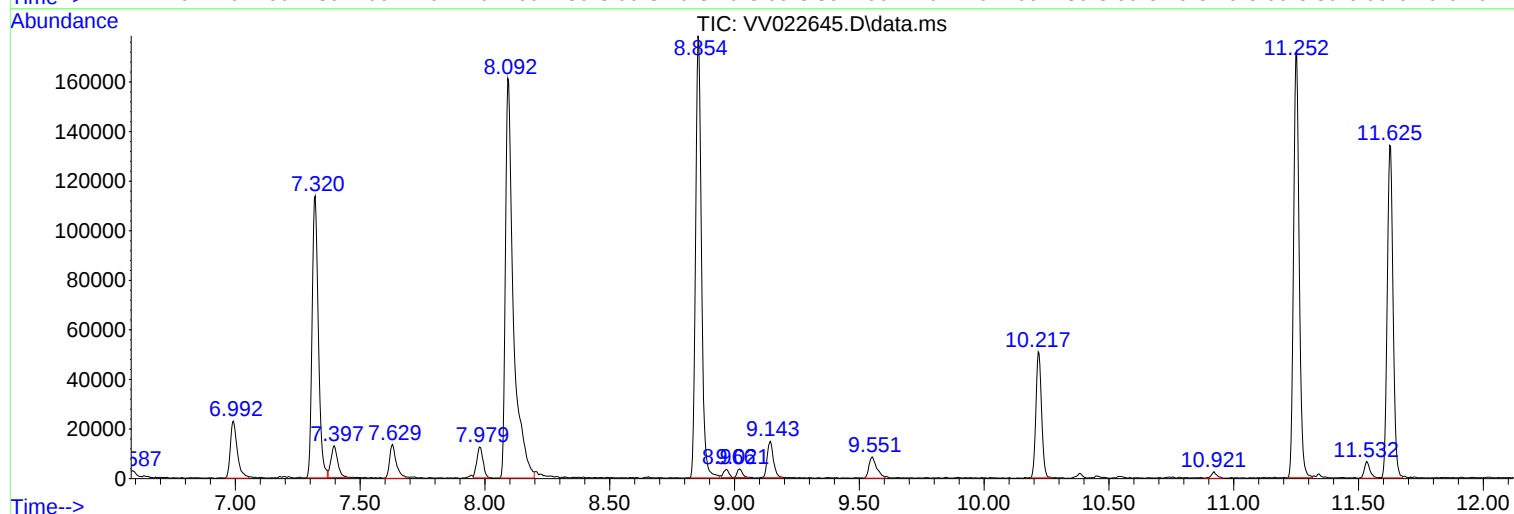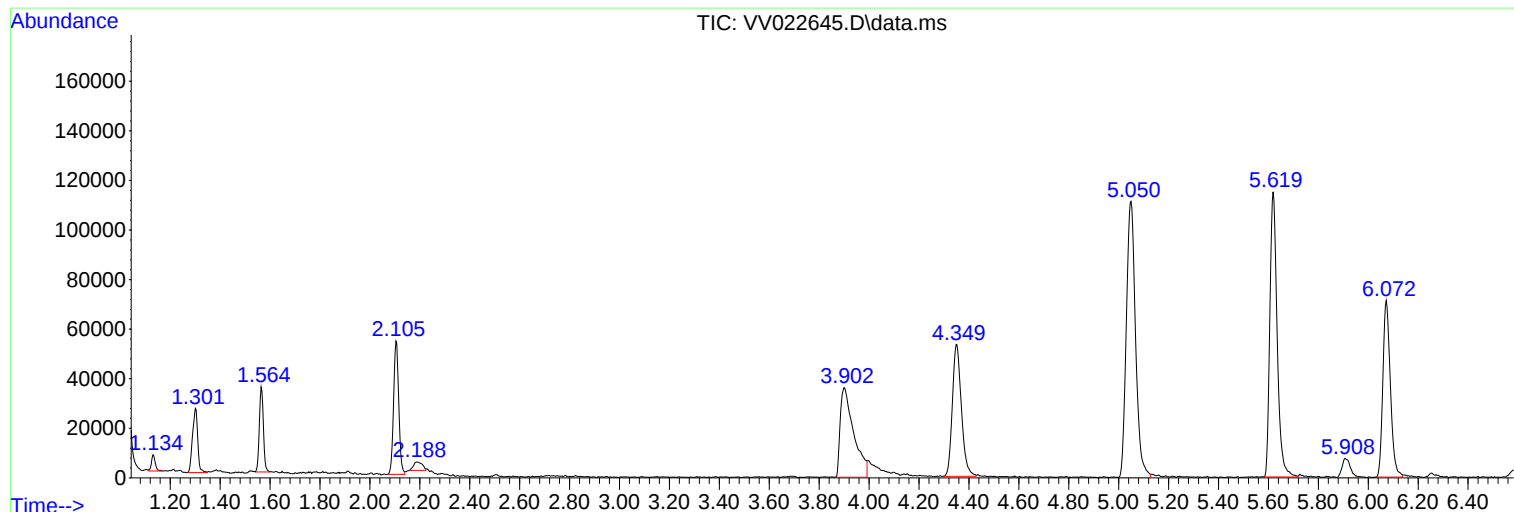

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022645.D
Acq On : 07 Oct 2021 01:27
Operator : SY/MD
Sample : M4050-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7C7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022645.D
Acq On : 07 Oct 2021 01:27
Operator : SY/MD
Sample : M4050-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7C7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
