

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
 Data File : VV022646.D
 Acq On : 07 Oct 2021 01:51
 Operator : SY/MD
 Sample : M4050-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7D8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022646.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	16	20	29	rVB2	10827	10534	2.43%	0.355%
2	1.304	74	82	90	rBV	26036	27354	6.30%	0.922%
3	1.565	155	163	173	rBV	35197	39636	9.13%	1.336%
4	2.108	321	332	345	rBV	49928	75284	17.34%	2.537%
5	3.889	876	886	923	rBV2	46639	159976	36.86%	5.391%
6	4.349	1013	1029	1048	rBV	50845	129425	29.82%	4.361%
7	5.050	1230	1247	1276	rBV2	108569	274095	63.15%	9.236%
8	5.619	1412	1424	1445	rBV	113297	227513	52.42%	7.666%
9	5.915	1503	1516	1543	rBV	221015	434051	100.00%	14.626%
10	6.072	1550	1565	1586	rBV2	70725	144695	33.34%	4.876%
11	6.992	1841	1851	1870	rBV3	22874	42789	9.86%	1.442%
12	7.320	1941	1953	1972	rBV	111913	196339	45.23%	6.616%
13	7.629	2039	2049	2067	rBV2	12744	23326	5.37%	0.786%
14	8.092	2182	2193	2234	rBV2	172103	350113	80.66%	11.797%
15	8.854	2419	2430	2455	rBV	172745	283162	65.24%	9.541%
16	10.217	2843	2854	2870	rVB	54910	86862	20.01%	2.927%
17	11.252	3165	3176	3194	rBV	163465	256108	59.00%	8.630%
18	11.625	3280	3292	3309	rBV	128921	201332	46.38%	6.784%
19	12.349	3509	3517	3525	rBV5	3834	5095	1.17%	0.172%




Sum of corrected areas: 2967689

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022646.D
Acq On : 07 Oct 2021 01:51
Operator : SY/MD
Sample : M4050-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7D8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

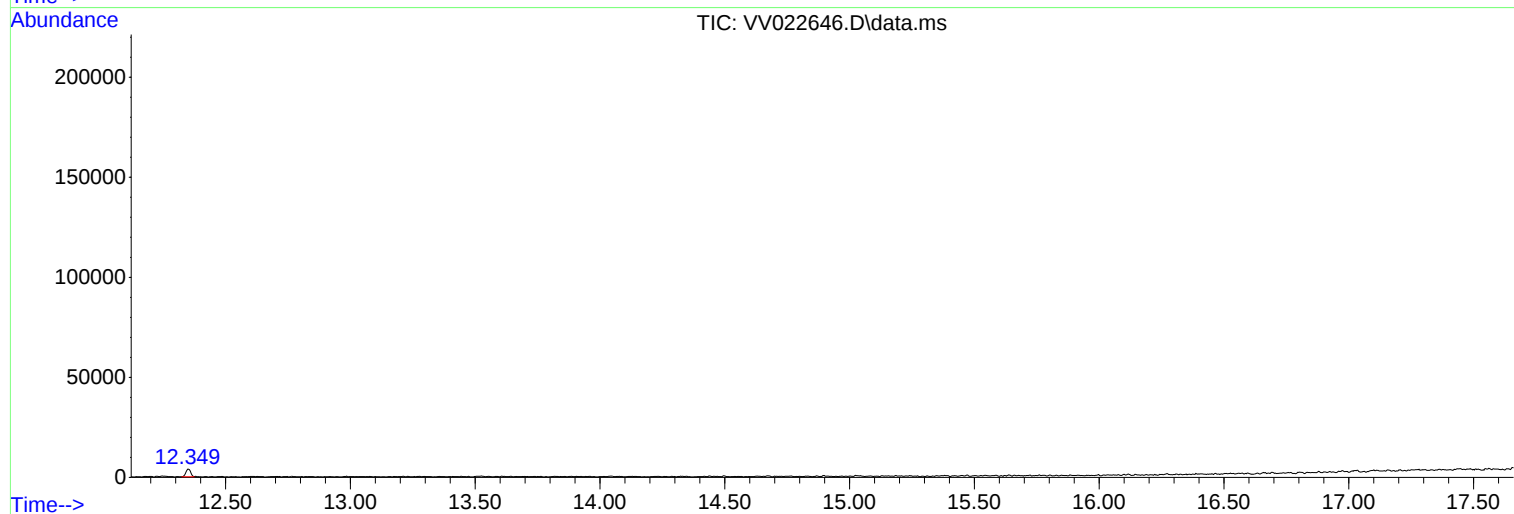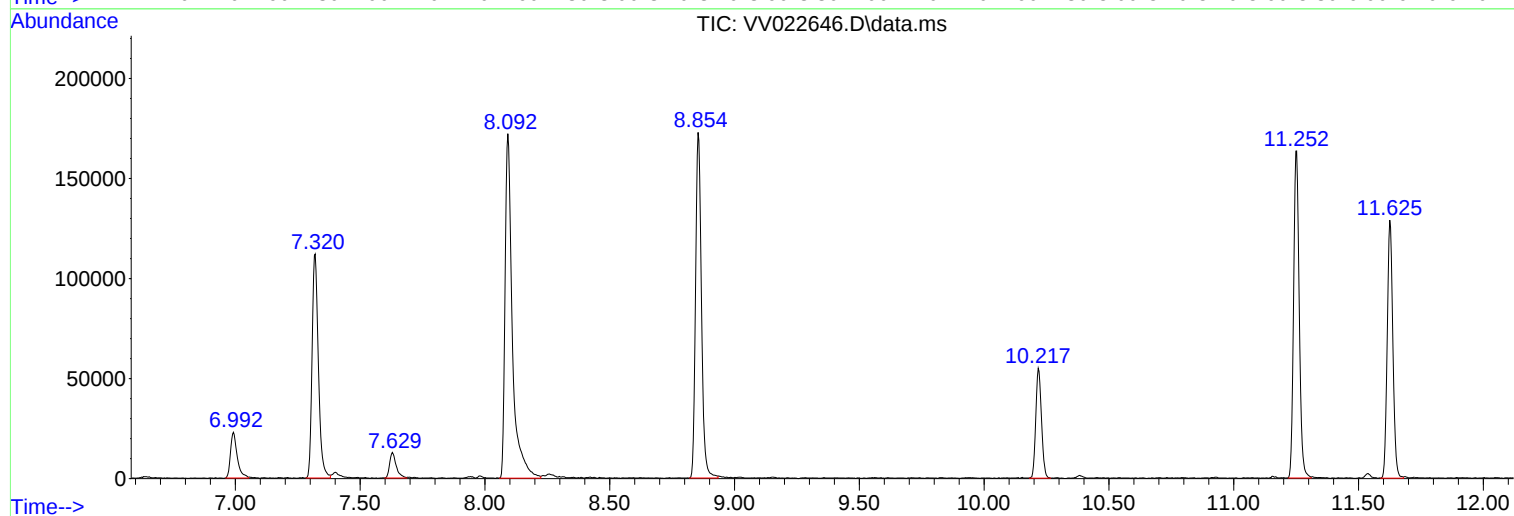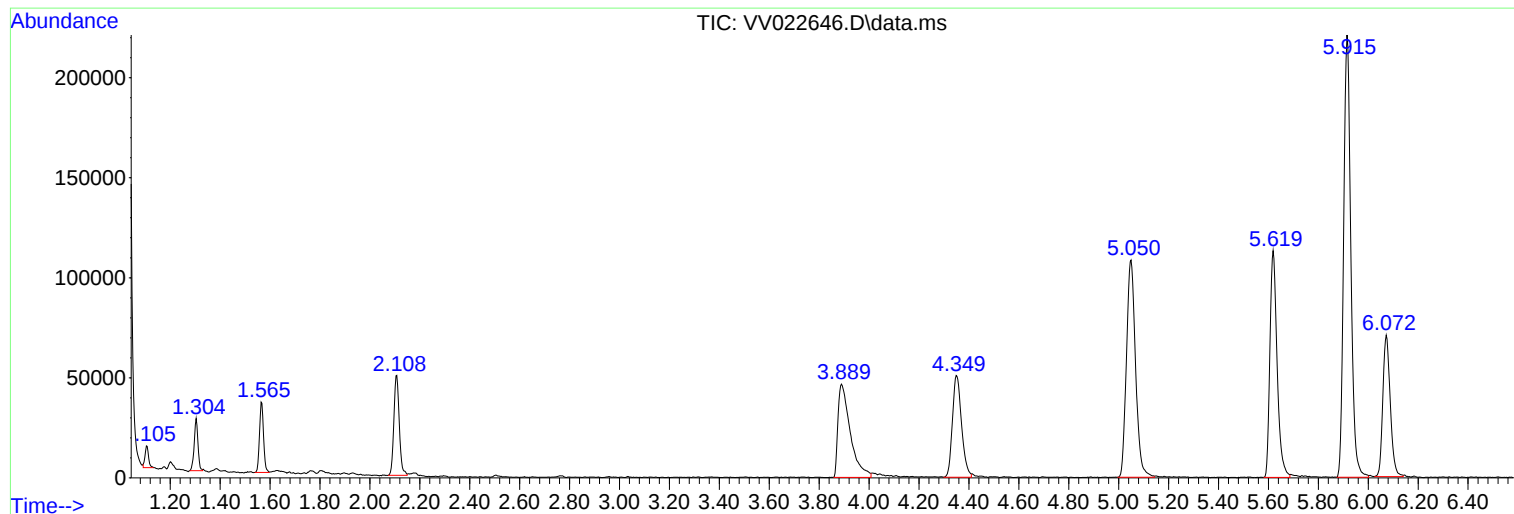

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022646.D
Acq On : 07 Oct 2021 01:51
Operator : SY/MD
Sample : M4050-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7D8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022646.D
Acq On : 07 Oct 2021 01:51
Operator : SY/MD
Sample : M4050-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7D8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
