

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
 Data File : VV022647.D
 Acq On : 07 Oct 2021 02:15
 Operator : SY/MD
 Sample : M4050-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7D9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022647.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	15	20	34	rVB	18737	19023	3.10%	0.585%
2	1.304	74	82	95	rVB2	27660	31968	5.21%	0.983%
3	1.565	156	163	174	rBV	35731	39201	6.39%	1.206%
4	2.108	319	332	344	rBV	52566	80888	13.19%	2.488%
5	2.169	346	351	364	rVB3	3438	6426	1.05%	0.198%
6	3.886	874	885	919	rBV	51965	169224	27.59%	5.205%
7	4.352	1014	1030	1051	rBV	52499	133089	21.70%	4.093%
8	5.047	1230	1246	1270	rBV2	110722	281490	45.89%	8.657%
9	5.619	1410	1424	1452	rBV	109930	226188	36.87%	6.956%
10	5.915	1502	1516	1548	rBV2	309337	613405	100.00%	18.865%
11	6.072	1552	1565	1583	rVV	70953	144712	23.59%	4.451%
12	6.992	1840	1851	1868	rBV3	23704	44797	7.30%	1.378%
13	7.320	1939	1953	1971	rBV	113908	201398	32.83%	6.194%
14	7.629	2039	2049	2073	rBV2	13892	25992	4.24%	0.799%
15	8.092	2182	2193	2228	rBV2	183861	361979	59.01%	11.133%
16	8.249	2234	2242	2252	rBV7	3403	6320	1.03%	0.194%
17	8.854	2419	2430	2452	rBV	169261	280577	45.74%	8.629%
18	10.217	2842	2854	2870	rBV	58280	90482	14.75%	2.783%
19	11.156	3137	3146	3156	rBV5	4797	7500	1.22%	0.231%
20	11.249	3164	3175	3191	rBV	164809	254998	41.57%	7.843%
21	11.625	3280	3292	3311	rBV	133402	211065	34.41%	6.491%
22	12.346	3508	3516	3529	rBV3	13880	20749	3.38%	0.638%




Sum of corrected areas: 3251471

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022647.D
Acq On : 07 Oct 2021 02:15
Operator : SY/MD
Sample : M4050-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
GB7D9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

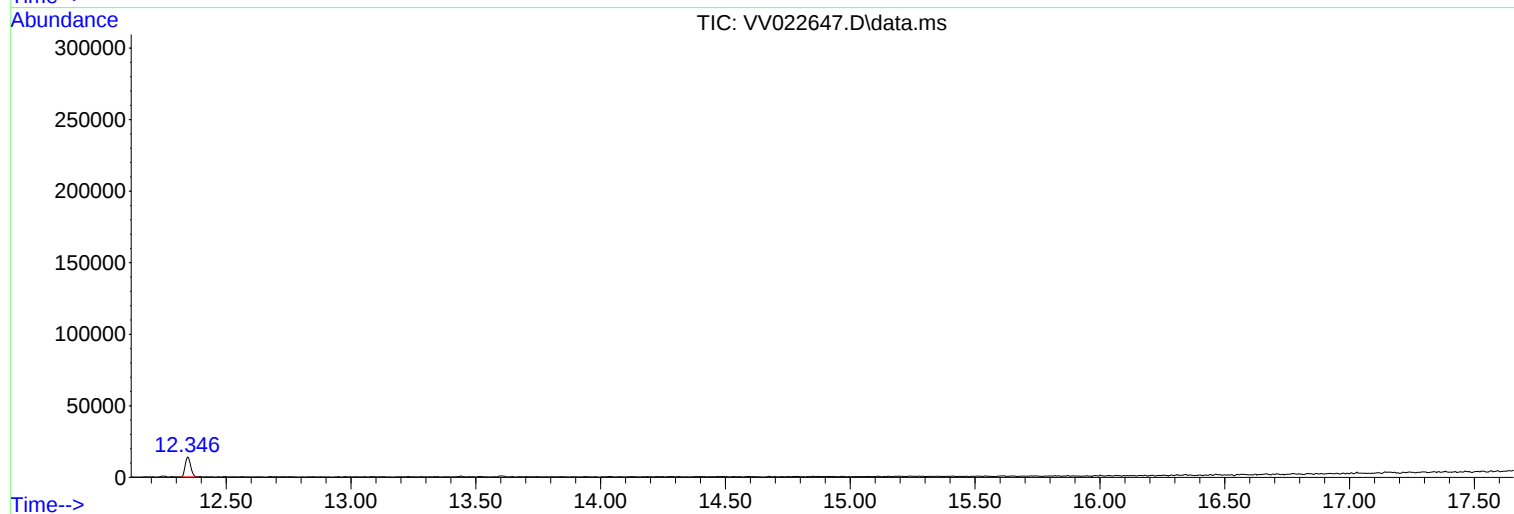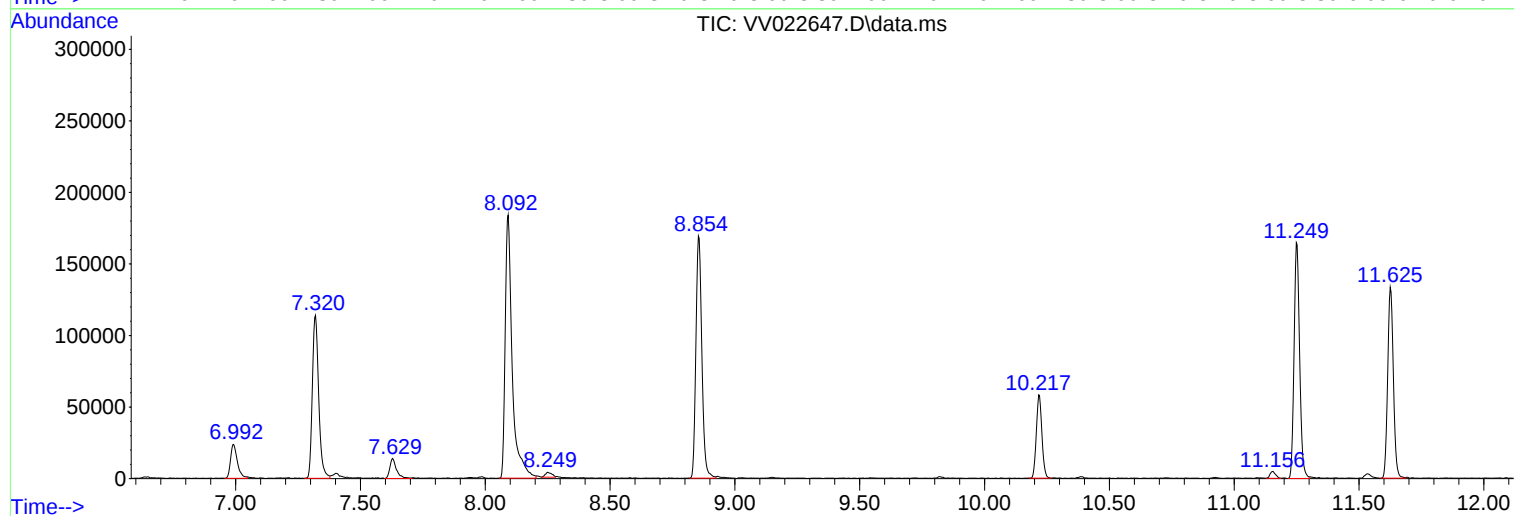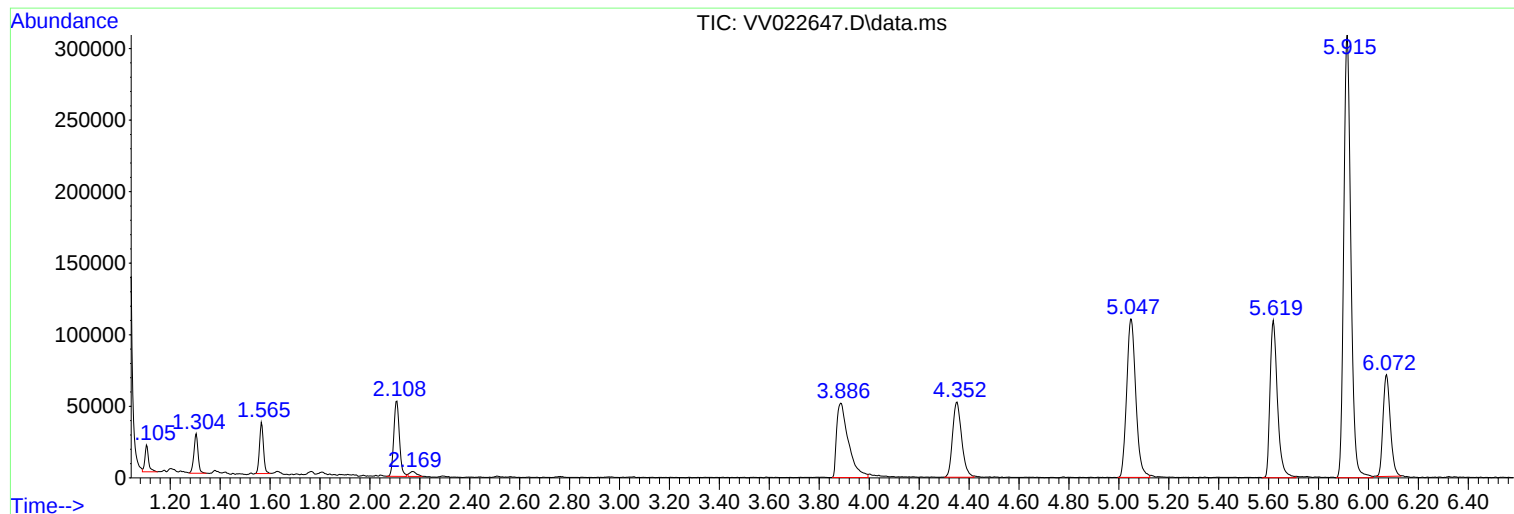

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022647.D
Acq On : 07 Oct 2021 02:15
Operator : SY/MD
Sample : M4050-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7D9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022647.D
Acq On : 07 Oct 2021 02:15
Operator : SY/MD
Sample : M4050-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7D9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
