

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
 Data File : VV022648.D
 Acq On : 07 Oct 2021 02:39
 Operator : SY/MD
 Sample : M4050-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7E0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022648.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	16	20	31	rVB	17820	17699	2.80%	0.548%
2	1.304	74	82	91	rVB2	28450	32973	5.22%	1.021%
3	1.564	155	163	173	rBV	31983	36394	5.76%	1.127%
4	2.108	322	332	346	rBV	52430	79361	12.56%	2.458%
5	2.172	346	352	368	rVB	3948	7705	1.22%	0.239%
6	3.883	875	884	921	rBV	52281	163981	25.95%	5.079%
7	4.352	1014	1030	1056	rBV2	51493	134126	21.23%	4.155%
8	5.050	1231	1247	1269	rBV2	107975	276574	43.78%	8.567%
9	5.619	1410	1424	1443	rBV	109856	225858	35.75%	6.996%
10	5.915	1503	1516	1542	rBV	327787	631804	100.00%	19.571%
11	6.072	1552	1565	1589	rVB2	68370	144883	22.93%	4.488%
12	6.992	1840	1851	1866	rBV2	22335	41742	6.61%	1.293%
13	7.320	1942	1953	1970	rBV	110712	194418	30.77%	6.022%
14	7.629	2037	2049	2061	rBV	13397	23767	3.76%	0.736%
15	8.092	2182	2193	2226	rBV2	178803	354391	56.09%	10.978%
16	8.256	2235	2244	2257	rVB7	3404	6777	1.07%	0.210%
17	8.854	2420	2430	2451	rBV	172274	280651	44.42%	8.693%
18	10.220	2844	2855	2869	rBV	55808	88343	13.98%	2.737%
19	11.156	3138	3146	3156	rBV4	4299	6442	1.02%	0.200%
20	11.252	3165	3176	3193	rBV	164301	256361	40.58%	7.941%
21	11.625	3280	3292	3312	rBV	130790	206566	32.69%	6.399%
22	12.345	3508	3516	3532	rVB4	11704	17496	2.77%	0.542%




Sum of corrected areas: 3228312

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022648.D
Acq On : 07 Oct 2021 02:39
Operator : SY/MD
Sample : M4050-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
GB7E0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

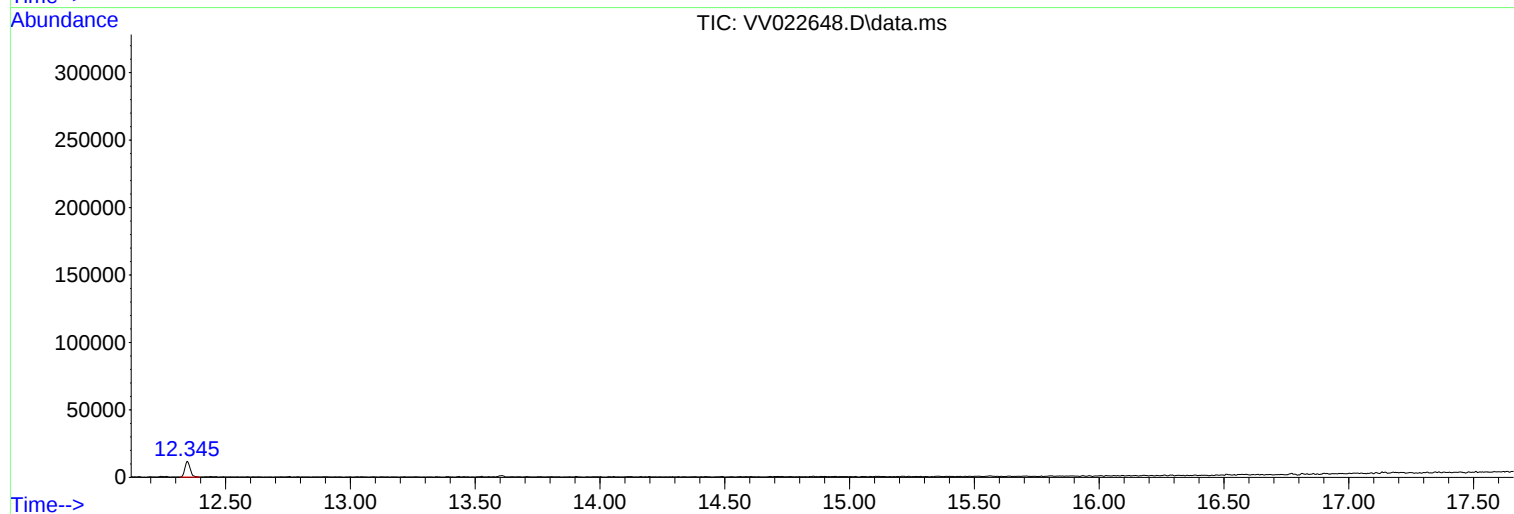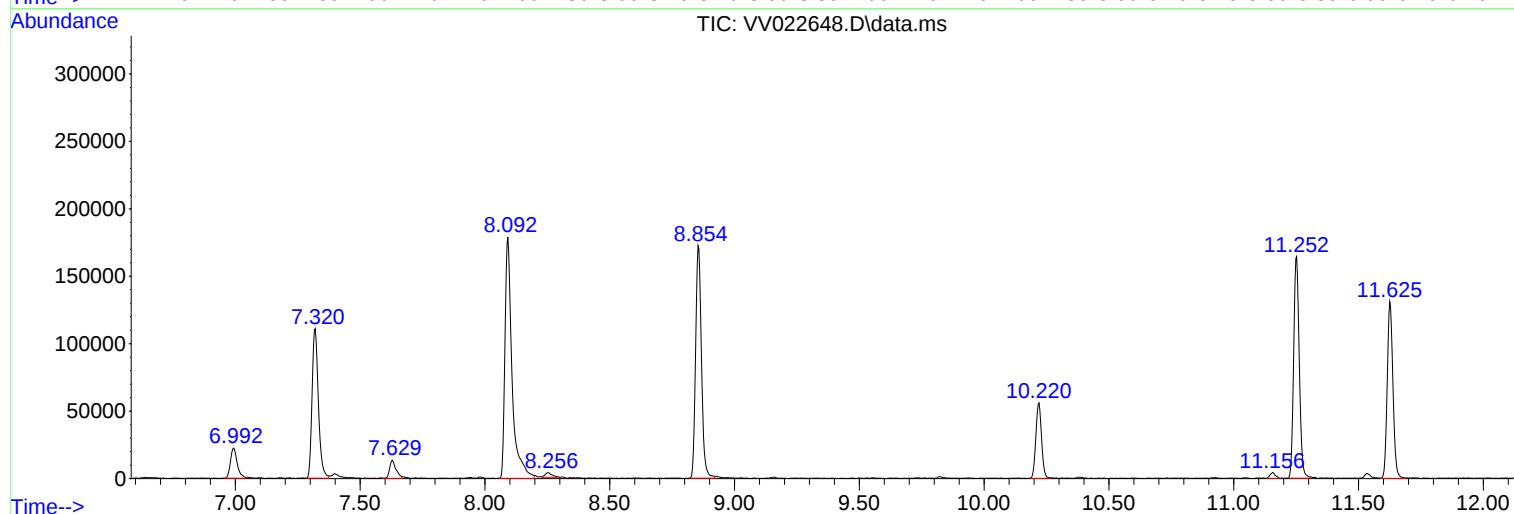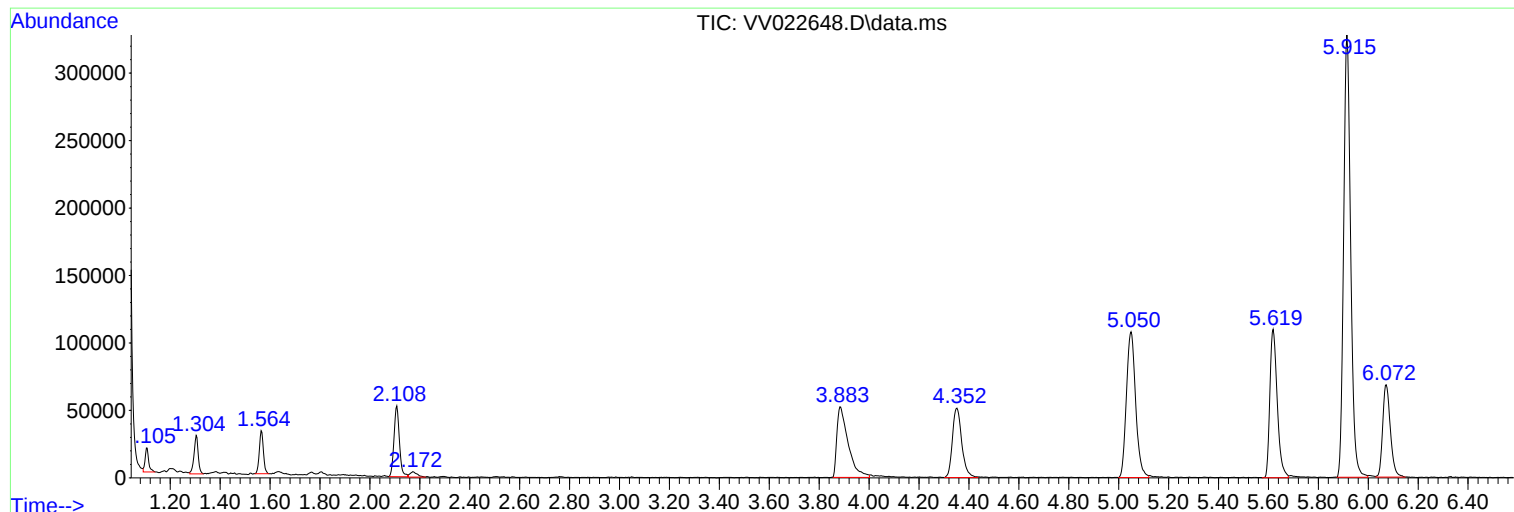

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022648.D
Acq On : 07 Oct 2021 02:39
Operator : SY/MD
Sample : M4050-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7E0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022648.D
Acq On : 07 Oct 2021 02:39
Operator : SY/MD
Sample : M4050-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7E0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
