

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
 Data File : VV022652.D
 Acq On : 07 Oct 2021 04:15
 Operator : SY/MD
 Sample : M4050-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7E4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022652.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	16	20	32	rVB	16677	16744	4.62%	0.596%
2	1.304	74	82	90	rVB2	28198	31476	8.68%	1.121%
3	1.568	156	164	173	rBV	33907	37974	10.47%	1.352%
4	2.108	322	332	345	rBV	52372	77592	21.39%	2.763%
5	3.905	876	891	924	rBV4	61791	219902	60.63%	7.830%
6	4.352	1013	1030	1061	rBV2	52584	134788	37.16%	4.799%
7	5.046	1232	1246	1267	rBV3	110438	278753	76.85%	9.925%
8	5.619	1412	1424	1441	rBV	112773	227815	62.81%	8.112%
9	5.918	1505	1517	1545	rBV	73548	154691	42.65%	5.508%
10	6.072	1552	1565	1592	rVB	71364	146001	40.25%	5.199%
11	6.992	1840	1851	1869	rBV	23430	43230	11.92%	1.539%
12	7.320	1941	1953	1970	rBV	110426	196668	54.22%	7.003%
13	7.628	2040	2049	2067	rBV3	13414	24220	6.68%	0.862%
14	7.982	2151	2159	2169	rVB4	3682	6036	1.66%	0.215%
15	8.091	2183	2193	2234	rBV3	176038	362722	100.00%	12.915%
16	8.853	2419	2430	2451	rBV	172805	285269	78.65%	10.157%
17	10.217	2843	2854	2873	rBV	55751	89078	24.56%	3.172%
18	11.249	3165	3175	3194	rBV	165521	258088	71.15%	9.190%
19	11.532	3256	3263	3276	rVB5	2724	4426	1.22%	0.158%
20	11.625	3281	3292	3308	rBV	130145	208074	57.36%	7.409%
21	12.345	3509	3516	3524	rBV4	3895	4948	1.36%	0.176%


Sum of corrected areas: 2808495

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022652.D
Acq On : 07 Oct 2021 04:15
Operator : SY/MD
Sample : M4050-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7E4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

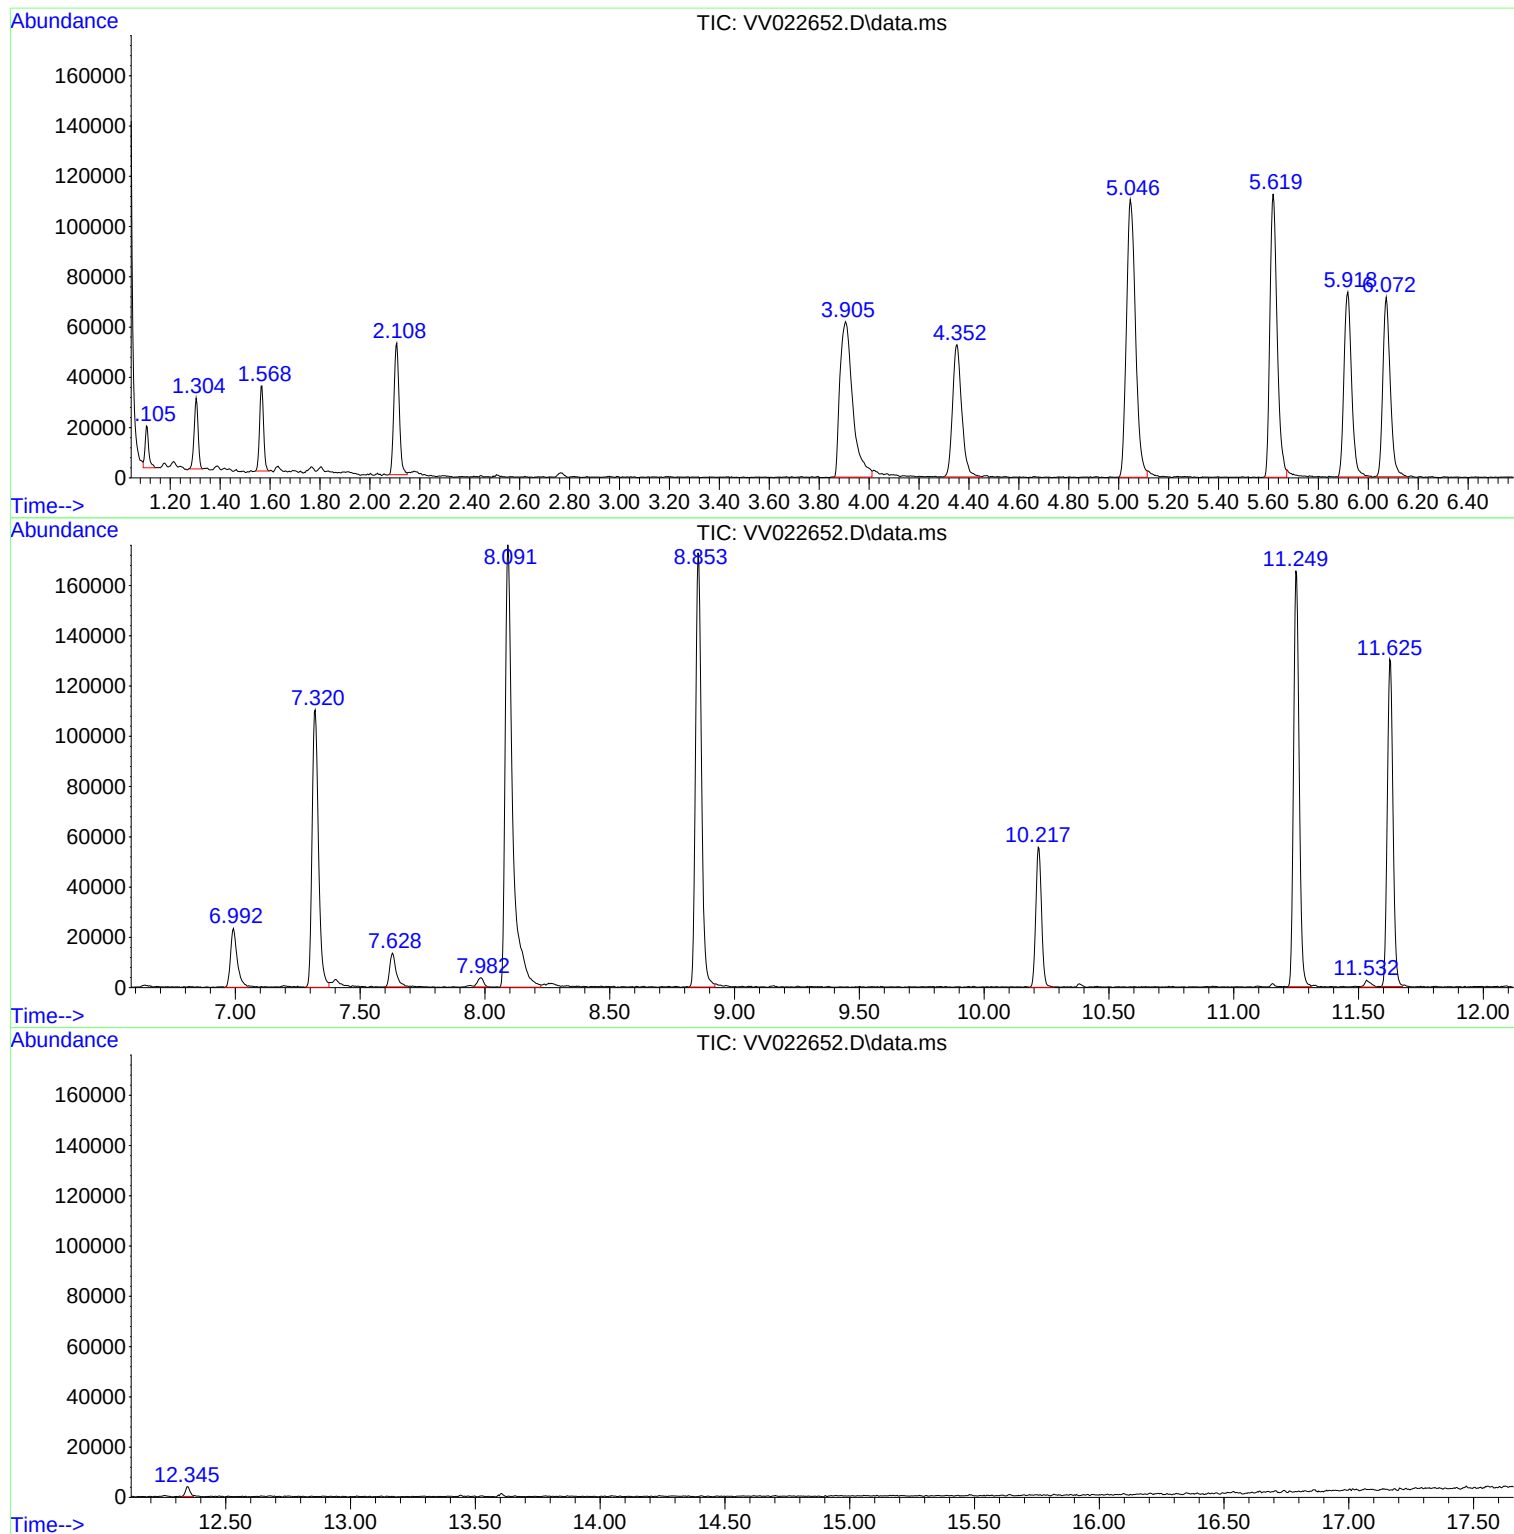

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022652.D
Acq On : 07 Oct 2021 04:15
Operator : SY/MD
Sample : M4050-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7E4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
Data File : VV022652.D
Acq On : 07 Oct 2021 04:15
Operator : SY/MD
Sample : M4050-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7E4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
