
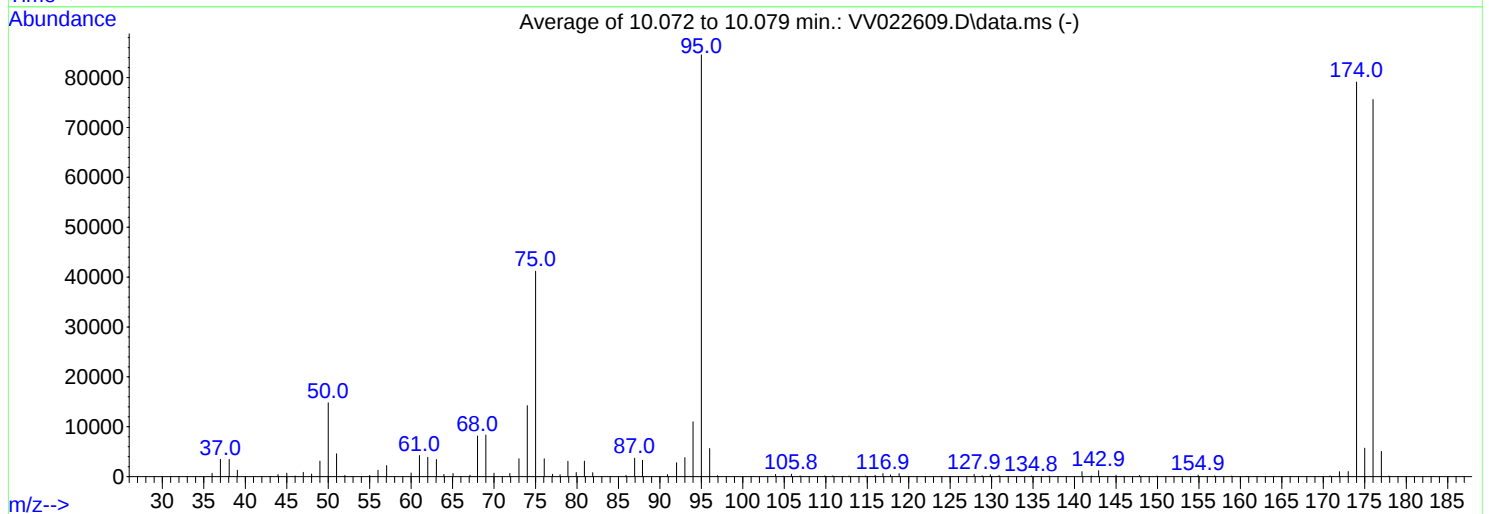


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100621\
 Data File : VV022609.D
 Acq On : 06 Oct 2021 09:28
 Operator : SY/MD
 Sample : BFB210
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB210

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Oct 08 02:23:59 2021

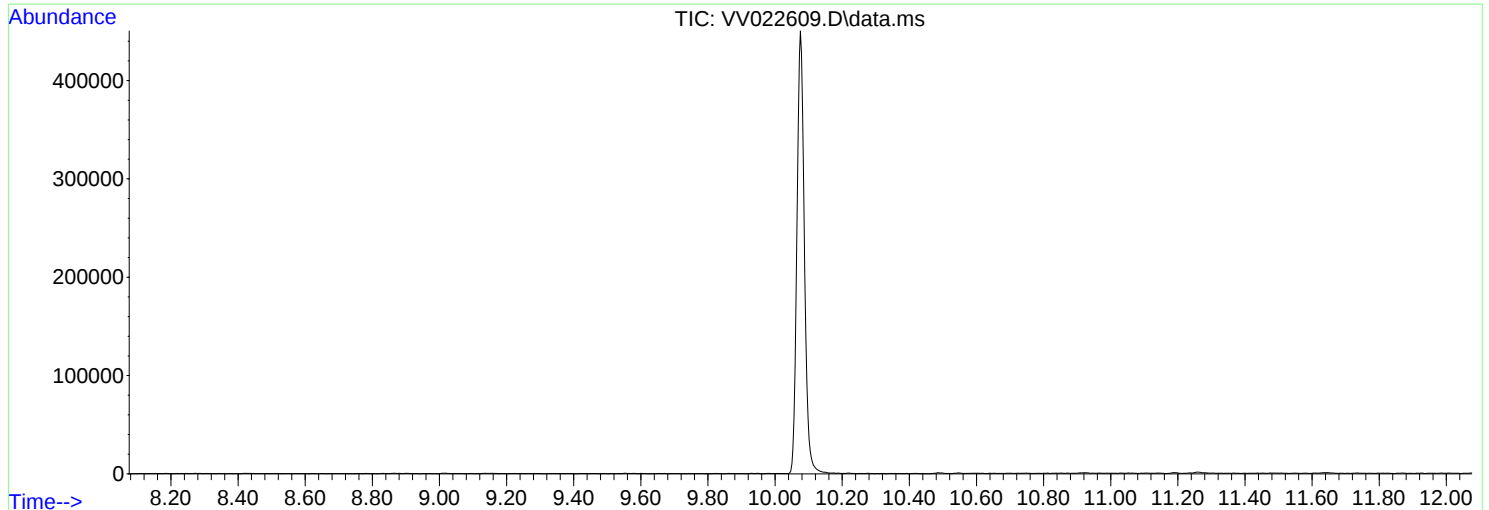

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	14833	PASS
75	95	30	80	48.7	41189	PASS
95	95	100	100	100.0	84555	PASS
96	95	5	9	6.7	5652	PASS
173	174	0.00	2	1.3	1031	PASS
174	95	50	120	93.5	79093	PASS
175	174	5	9	7.2	5704	PASS
176	174	95	105	95.6	75584	PASS
177	176	5	10	6.7	5076	PASS

Scan 2797 (10.034 min): VV022609.D\data.ms
BFB210

m/z	Abundance
40.10	115.0
43.90	198.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210

m/z	Abundance
36.00	680.0
37.00	3503.0
38.10	3631.0
39.10	1298.0
40.10	221.0
43.10	104.0
44.00	644.0
45.00	675.0
46.00	149.0
47.00	852.0
48.00	561.0
49.00	2958.0
50.00	14831.0
51.00	4534.0
52.00	260.0
52.80	110.0
55.00	250.0
56.00	1228.0
57.00	2208.0
58.00	111.0
60.00	735.0
61.00	4214.0
62.00	3953.0
63.00	3365.0
64.00	454.0
65.10	709.0
65.90	128.0
67.10	278.0
68.00	8093.0
69.00	8612.0
70.00	645.0
71.90	569.0
73.00	3573.0
74.00	13923.0
75.00	41184.0
76.10	3610.0
77.10	482.0
78.00	435.0
78.90	3129.0
79.90	846.0
80.90	3069.0
81.90	757.0
85.90	260.0
86.90	3697.0
87.90	3405.0
90.90	352.0
92.00	2811.0
93.00	3801.0
94.00	10730.0
95.00	82688.0
96.00	5447.0
96.90	195.0
104.00	410.0
105.00	100.0
105.80	539.0
106.90	129.0
109.90	146.0
110.90	175.0
112.80	141.0
114.80	106.0
115.90	265.0
116.90	571.0
117.80	363.0
118.80	571.0
123.90	120.0
127.90	464.0
128.90	183.0
129.90	386.0
130.90	212.0
134.80	135.0
136.90	120.0
140.90	929.0
142.00	112.0
142.90	1152.0
145.00	275.0
146.00	123.0
147.90	251.0
150.00	106.0
154.90	268.0
156.90	144.0
158.90	119.0
160.80	102.0
170.80	144.0
171.90	944.0
173.00	967.0
174.00	76248.0
175.00	5648.0
176.00	72712.0
177.00	5003.0
178.10	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210

m/z	Abundance
36.00	701.0
37.00	3538.0
38.00	3573.0
39.10	1342.0
40.10	204.0
44.00	662.0
45.00	766.0
46.00	147.0
47.00	886.0
48.00	533.0
49.00	3257.0
50.00	15495.0
51.00	4692.0
52.00	253.0
55.00	270.0
56.00	1347.0
57.00	2274.0
60.00	771.0
61.00	4449.0
62.00	4011.0
63.00	3609.0
63.90	466.0
65.00	671.0
67.10	303.0
68.00	8435.0
69.00	8609.0
70.00	731.0
71.90	706.0
73.00	3702.0
74.00	14745.0
75.00	42656.0
76.00	3726.0
77.00	484.0
78.00	412.0
78.90	3174.0
79.90	858.0
80.90	3221.0
81.90	831.0
82.90	108.0
85.90	273.0
87.00	3804.0
87.90	3320.0
90.90	430.0
92.00	2903.0
93.00	3962.0
94.00	11546.0
95.00	87792.0
96.00	5838.0
97.00	188.0
103.90	445.0
105.00	105.0
105.90	494.0
106.90	162.0
109.90	156.0
110.90	177.0
112.10	101.0
112.80	142.0
114.80	127.0
115.90	286.0
116.90	617.0
117.80	360.0
118.90	620.0
123.90	129.0
127.90	468.0
128.80	224.0
129.90	407.0
130.90	222.0
134.80	166.0
137.00	149.0
140.90	1033.0
142.10	120.0
142.90	1235.0
144.00	116.0
145.00	308.0
145.90	108.0
147.90	281.0
149.90	122.0
154.90	331.0
156.90	161.0
158.90	126.0
160.80	109.0
170.80	151.0
172.00	1058.0
173.00	1084.0
174.00	82032.0
175.00	5964.0
176.00	78384.0
177.00	5310.0
177.90	132.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210

m/z	Abundance
36.00	666.0
37.00	3338.0
38.00	3151.0
39.00	1207.0
40.00	166.0
44.00	590.0
45.00	727.0
46.00	130.0
47.00	837.0
48.00	472.0
49.00	3131.0
50.00	14172.0
51.00	4496.0
52.00	222.0
55.00	254.0
56.00	1292.0
57.10	2200.0
60.00	745.0
61.00	4018.0
62.00	3661.0
63.10	3299.0
64.00	410.0
65.00	577.0
67.10	254.0
68.00	7944.0
69.00	7769.0
70.00	734.0
71.90	638.0
73.00	3552.0
74.00	14024.0
75.00	39728.0
76.00	3457.0
77.00	503.0
77.90	343.0
78.90	2906.0
79.90	812.0
80.90	3081.0
81.90	792.0
82.90	126.0
85.90	260.0
87.00	3535.0
87.90	3090.0
90.90	453.0
92.00	2619.0
93.00	3673.0
94.00	10767.0
95.00	83184.0
96.00	5670.0
97.00	207.0
103.90	466.0
104.80	133.0
105.90	426.0
106.90	168.0
109.90	142.0
110.80	138.0
112.10	106.0
112.80	109.0
113.00	110.0
114.80	115.0
116.00	291.0
116.90	630.0
117.80	322.0
118.90	597.0
124.90	101.0
127.90	461.0
128.80	223.0
129.80	354.0
130.90	215.0
134.80	173.0
137.00	170.0
140.90	1058.0
142.10	124.0
142.90	1206.0
144.00	107.0
145.00	276.0
145.90	105.0
147.80	276.0
149.90	120.0
154.90	339.0
156.90	192.0
158.90	113.0
170.80	157.0
172.00	1031.0
173.00	1041.0
174.00	79000.0
175.00	5500.0
176.00	75656.0
177.00	4916.0
177.80	157.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210