

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100623\
 Data File : VV032292.D
 Acq On : 06 Oct 2023 11:18
 Operator : SY/MD
 Sample : VV1006WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK365

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032292.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rVB	49846	54549	15.29%	1.981%
2	1.532	146	153	165	rVB	47155	54360	15.24%	1.974%
3	2.060	307	317	331	rBV	77190	111856	31.35%	4.062%
4	2.172	345	352	363	rVB3	3500	6373	1.79%	0.231%
5	2.449	427	438	451	rBV2	7446	12363	3.47%	0.449%
6	3.805	850	860	890	rBV	40338	126580	35.48%	4.596%
7	4.252	981	999	1024	rBV2	53198	144405	40.47%	5.244%
8	4.960	1201	1219	1239	rBV2	129118	331282	92.85%	12.030%
9	5.539	1387	1399	1416	rBV	91562	191440	53.66%	6.952%
10	5.834	1480	1491	1503	rBV5	3926	8319	2.33%	0.302%
11	5.992	1529	1540	1554	rBV	73314	154584	43.33%	5.613%
12	6.918	1819	1828	1855	rBV	29174	61881	17.34%	2.247%
13	7.249	1920	1931	1961	rBV	144816	275945	77.34%	10.020%
14	7.561	2019	2028	2049	rBV2	16698	35323	9.90%	1.283%
15	8.034	2163	2175	2217	rBV	159742	356786	100.00%	12.956%
16	8.789	2399	2410	2436	rBV	147348	259438	72.72%	9.421%
17	10.159	2825	2836	2850	rBV	56501	90450	25.35%	3.284%
18	11.188	3143	3156	3177	rBV	148363	238478	66.84%	8.660%
19	11.564	3262	3273	3290	rBV	147345	235705	66.06%	8.559%
20	13.451	3852	3860	3867	rBV2	2777	3780	1.06%	0.137%




Sum of corrected areas: 2753897

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100623\
Data File : VV032292.D
Acq On : 06 Oct 2023 11:18
Operator : SY/MD
Sample : VV1006WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK365

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

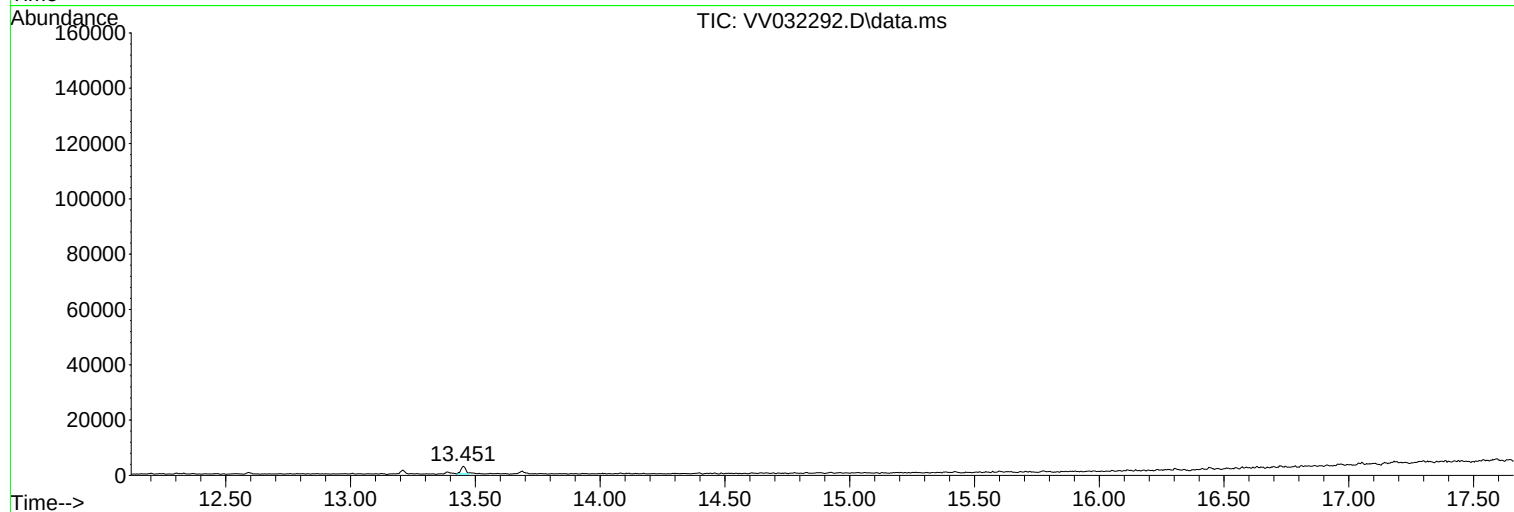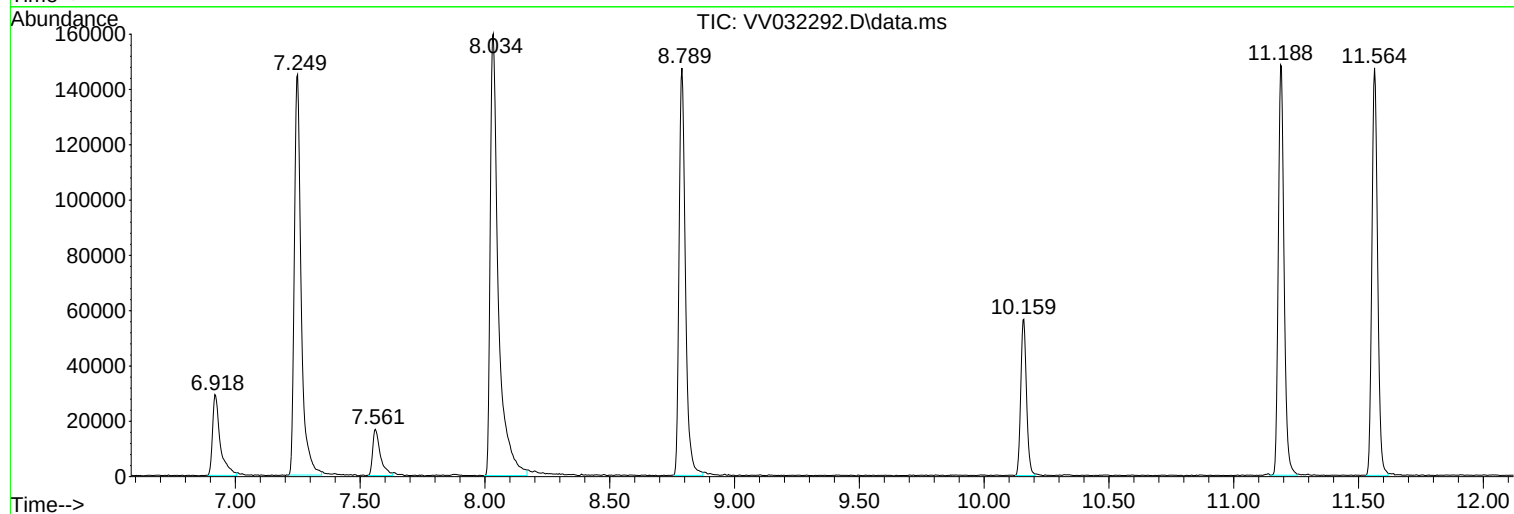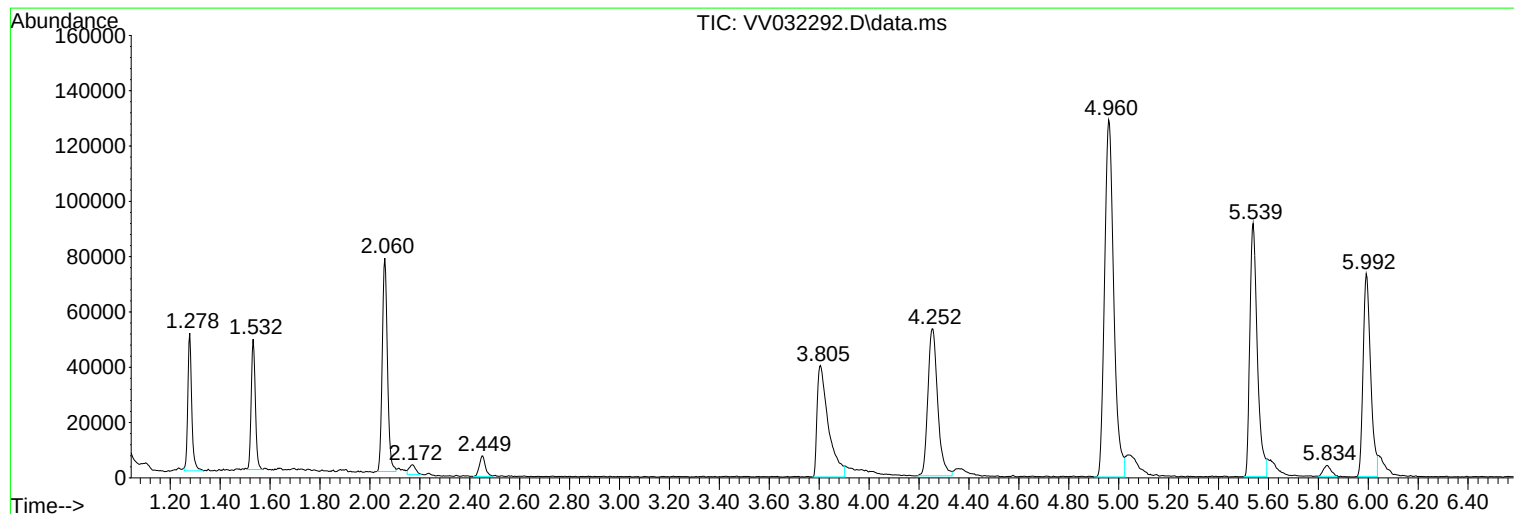

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100623\
Data File : VV032292.D
Acq On : 06 Oct 2023 11:18
Operator : SY/MD
Sample : VV1006WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK365

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100623\
Data File : VV032292.D
Acq On : 06 Oct 2023 11:18
Operator : SY/MD
Sample : VV1006WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK365

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc