

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100623\
 Data File : VV032299.D
 Acq On : 06 Oct 2023 14:15
 Operator : SY/MD
 Sample : 04744-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032299.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	18	22	32	rVB	3347	5152	1.49%	0.191%
2	1.278	67	74	88	rVB	42136	45004	12.98%	1.664%
3	1.532	145	153	165	rBV	42481	50036	14.44%	1.850%
4	2.060	307	317	334	rBV	64616	96448	27.83%	3.566%
5	2.182	347	355	365	rVB2	4867	9488	2.74%	0.351%
6	2.445	431	437	449	rVB3	2509	3834	1.11%	0.142%
7	3.806	851	860	891	rBV	40512	125776	36.29%	4.651%
8	4.256	983	1000	1022	rBV	50786	135733	39.16%	5.019%
9	4.963	1203	1220	1238	rBV2	117150	300414	86.67%	11.108%
10	5.539	1387	1399	1416	rBV	101209	207941	59.99%	7.689%
11	5.834	1481	1491	1501	rBV3	2180	4813	1.39%	0.178%
12	5.995	1526	1541	1554	rBV	69342	143881	41.51%	5.320%
13	6.921	1818	1829	1861	rBV	27782	60936	17.58%	2.253%
14	7.246	1920	1930	1968	rBV	134524	259362	74.83%	9.590%
15	7.561	2020	2028	2055	rBV2	15916	33975	9.80%	1.256%
16	8.030	2161	2174	2214	rBV	165512	346622	100.00%	12.817%
17	8.789	2398	2410	2437	rBV	164520	286100	82.54%	10.579%
18	10.159	2825	2836	2850	rBV	54049	89739	25.89%	3.318%
19	11.188	3145	3156	3174	rBV	169865	268249	77.39%	9.919%
20	11.564	3256	3273	3291	rBV	145216	230955	66.63%	8.540%




Sum of corrected areas: 2704458

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100623\
Data File : VV032299.D
Acq On : 06 Oct 2023 14:15
Operator : SY/MD
Sample : 04744-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

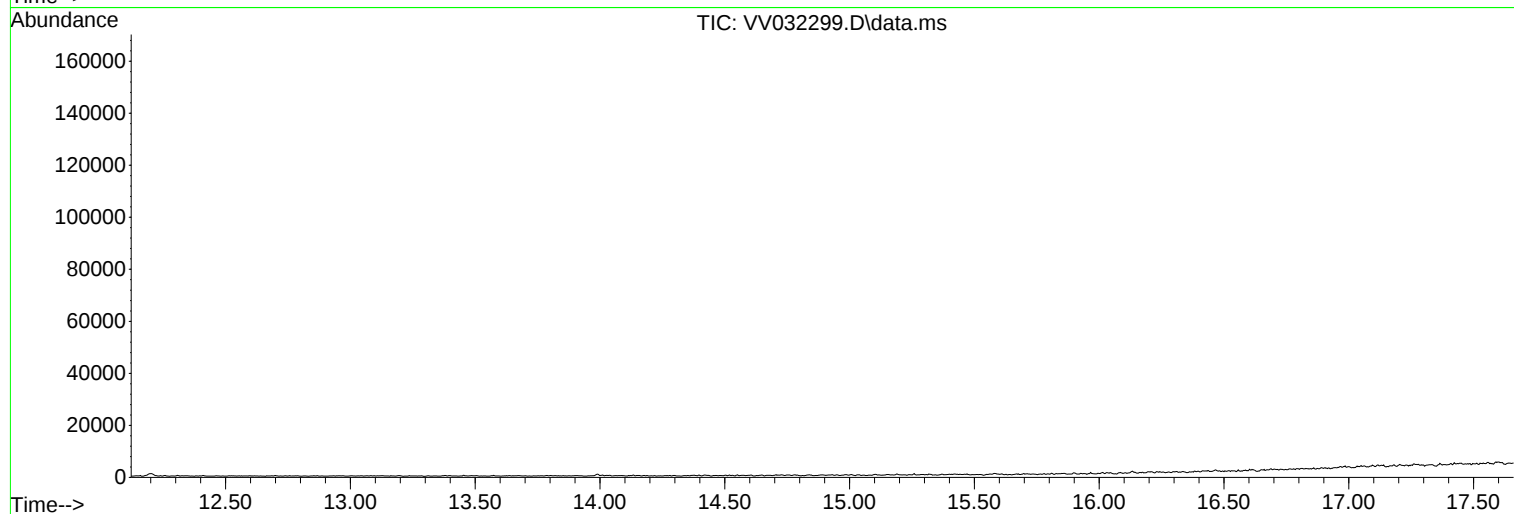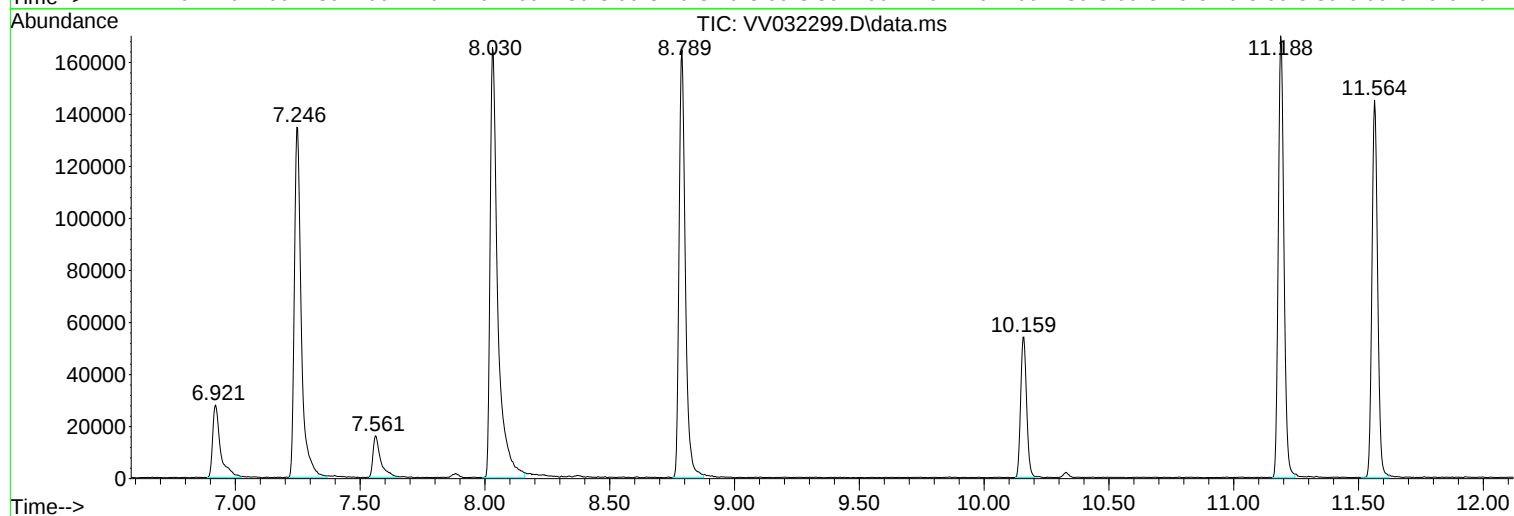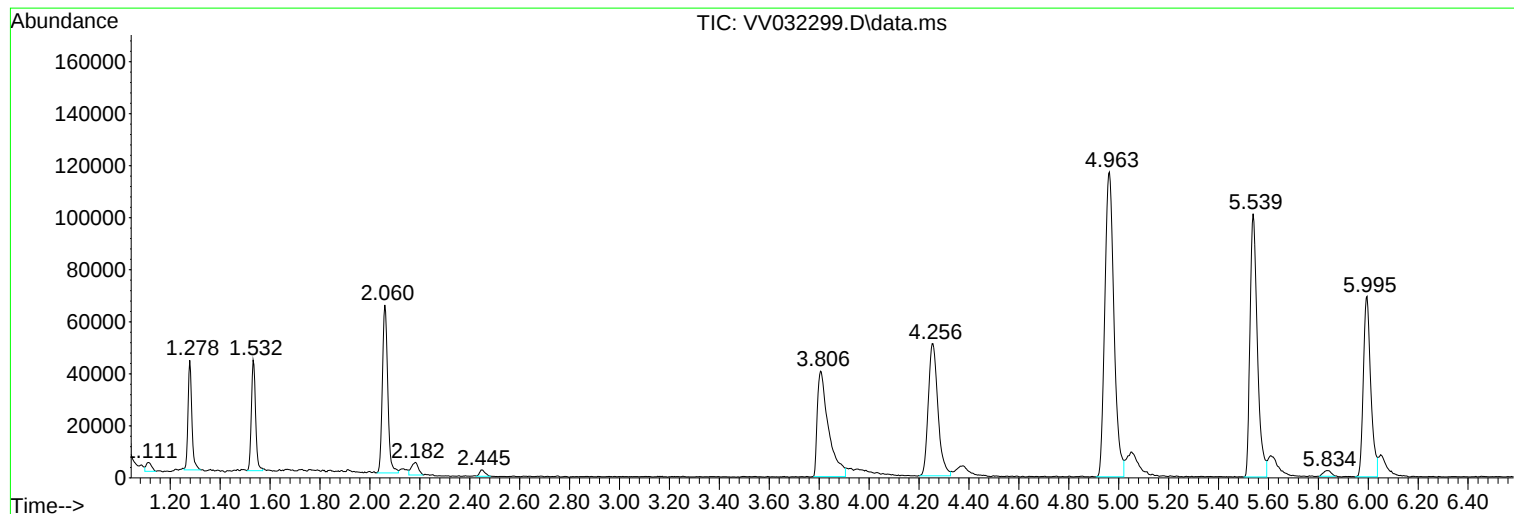

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100623\
Data File : VV032299.D
Acq On : 06 Oct 2023 14:15
Operator : SY/MD
Sample : 04744-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100623\
Data File : VV032299.D
Acq On : 06 Oct 2023 14:15
Operator : SY/MD
Sample : 04744-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc