

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100623\
 Data File : VV032301.D
 Acq On : 06 Oct 2023 15:04
 Operator : SY/MD
 Sample : 04748-06DL 40X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX879DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032301.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	19	24	32	rVB	4745	6366	1.34%	0.188%
2	1.278	66	74	87	rBV	43829	47891	10.04%	1.413%
3	1.532	146	153	167	rVB	43019	50740	10.64%	1.497%
4	2.060	308	317	332	rBV	66027	96944	20.33%	2.861%
5	2.182	346	355	368	rVB2	5558	10613	2.23%	0.313%
6	2.449	429	438	451	rBV	8103	14416	3.02%	0.425%
7	3.815	852	863	888	rBV	46862	151861	31.85%	4.481%
8	4.253	984	999	1020	rBV	52651	139432	29.24%	4.115%
9	4.368	1025	1035	1056	rVB2	4367	13394	2.81%	0.395%
10	4.960	1204	1219	1238	rBV3	122024	311816	65.40%	9.202%
11	5.539	1386	1399	1415	rBV	104779	214381	44.96%	6.326%
12	5.834	1479	1491	1505	rBV	233279	476796	100.00%	14.070%
13	5.899	1506	1511	1529	rVB3	25546	51600	10.82%	1.523%
14	5.992	1529	1540	1555	rBV	70512	144846	30.38%	4.274%
15	6.921	1818	1829	1841	rBV	28820	55915	11.73%	1.650%
16	7.246	1916	1930	1969	rBV	139045	272240	57.10%	8.034%
17	7.564	2018	2029	2054	rBV2	17058	36811	7.72%	1.086%
18	8.034	2165	2175	2205	rBV	178410	376066	78.87%	11.098%
19	8.789	2399	2410	2440	rBV	172841	299421	62.80%	8.836%
20	10.159	2822	2836	2857	rBV	60242	97520	20.45%	2.878%
21	11.188	3146	3156	3177	rBV	180087	279518	58.62%	8.249%
22	11.564	3262	3273	3291	rBV	151894	240105	50.36%	7.085%




Sum of corrected areas: 3388692

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100623\
Data File : VV032301.D
Acq On : 06 Oct 2023 15:04
Operator : SY/MD
Sample : 04748-06DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX879DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

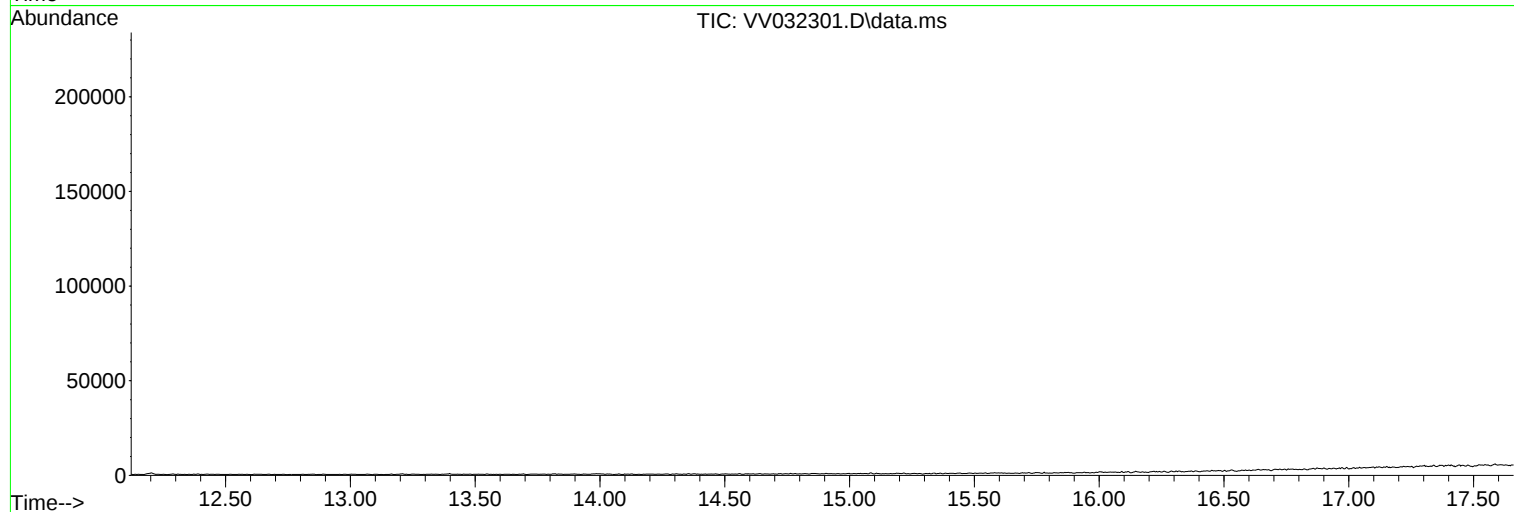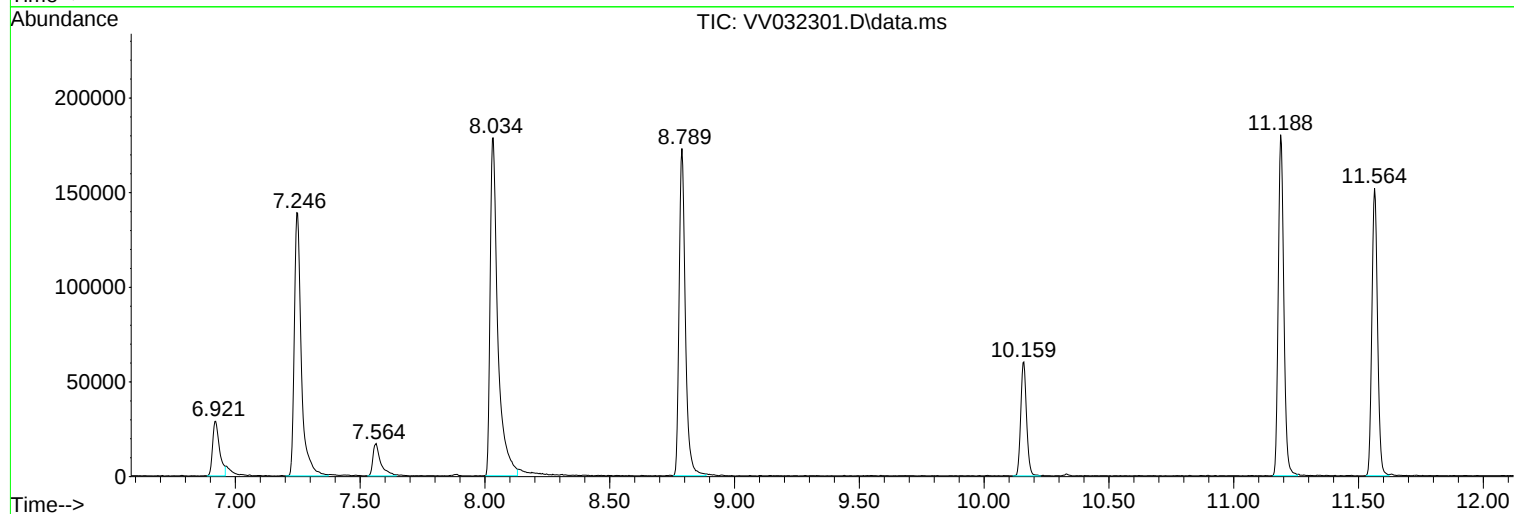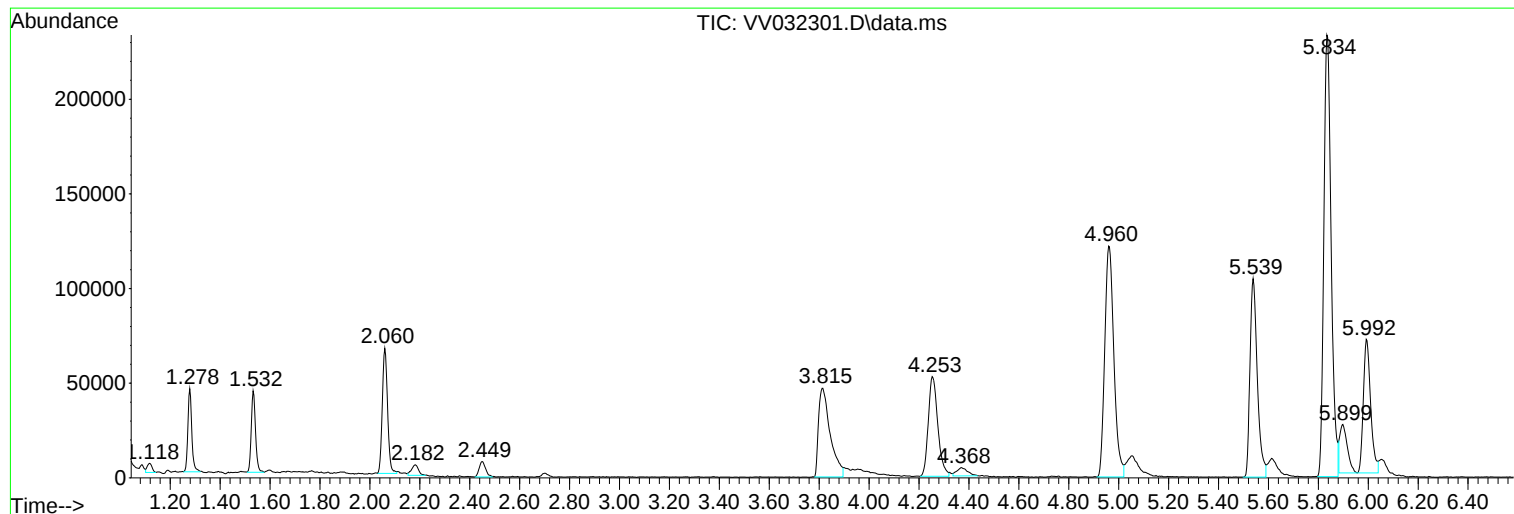

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100623\
Data File : VV032301.D
Acq On : 06 Oct 2023 15:04
Operator : SY/MD
Sample : 04748-06DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX879DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100623\
Data File : VV032301.D
Acq On : 06 Oct 2023 15:04
Operator : SY/MD
Sample : 04748-06DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX879DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc