

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100623\
 Data File : VV032305.D
 Acq On : 06 Oct 2023 16:42
 Operator : SY/MD
 Sample : 04748-26DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX864DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032305.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	9	14	19	rVV	10865	9724	2.69%	0.312%
2	1.121	20	25	33	rVB	8643	10797	2.99%	0.346%
3	1.192	41	47	55	rBV	5561	5203	1.44%	0.167%
4	1.278	66	74	89	rBV	43630	48861	13.53%	1.566%
5	1.532	146	153	165	rVV	40376	47485	13.15%	1.522%
6	1.600	168	174	180	rVB6	2692	3693	1.02%	0.118%
7	2.060	306	317	330	rBV	61738	90855	25.16%	2.912%
8	2.185	349	356	366	rVB2	5239	9063	2.51%	0.291%
9	2.449	428	438	448	rBV2	9436	15634	4.33%	0.501%
10	3.799	849	858	892	rBV2	46027	139385	38.60%	4.468%
11	4.252	983	999	1021	rBV	47951	125273	34.69%	4.016%
12	4.375	1025	1037	1058	rVB3	4705	13782	3.82%	0.442%
13	4.960	1205	1219	1238	rBV3	110120	284854	78.88%	9.131%
14	5.539	1387	1399	1416	rBV2	102573	207094	57.35%	6.638%
15	5.619	1417	1424	1438	rVB2	8449	20187	5.59%	0.647%
16	5.834	1479	1491	1505	rBV	165286	332650	92.12%	10.663%
17	5.902	1506	1512	1529	rVB3	19244	40564	11.23%	1.300%
18	5.995	1529	1541	1554	rBV2	62988	131271	36.35%	4.208%
19	6.918	1819	1828	1854	rBV	26629	59498	16.48%	1.907%
20	7.249	1919	1931	1967	rBV	126619	247608	68.57%	7.937%
21	7.561	2017	2028	2061	rBB	15101	33703	9.33%	1.080%
22	7.879	2116	2127	2139	rVB3	2173	3792	1.05%	0.122%
23	8.030	2162	2174	2217	rBV	173714	361107	100.00%	11.575%
24	8.789	2398	2410	2436	rBV	167992	291525	80.73%	9.345%
25	10.159	2824	2836	2861	rVB	56829	92383	25.58%	2.961%
26	11.188	3145	3156	3182	rBV	177239	272345	75.42%	8.730%
27	11.564	3261	3273	3292	rBV	136654	221387	61.31%	7.096%




Sum of corrected areas: 3119723

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100623\
Data File : VV032305.D
Acq On : 06 Oct 2023 16:42
Operator : SY/MD
Sample : 04748-26DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX864DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

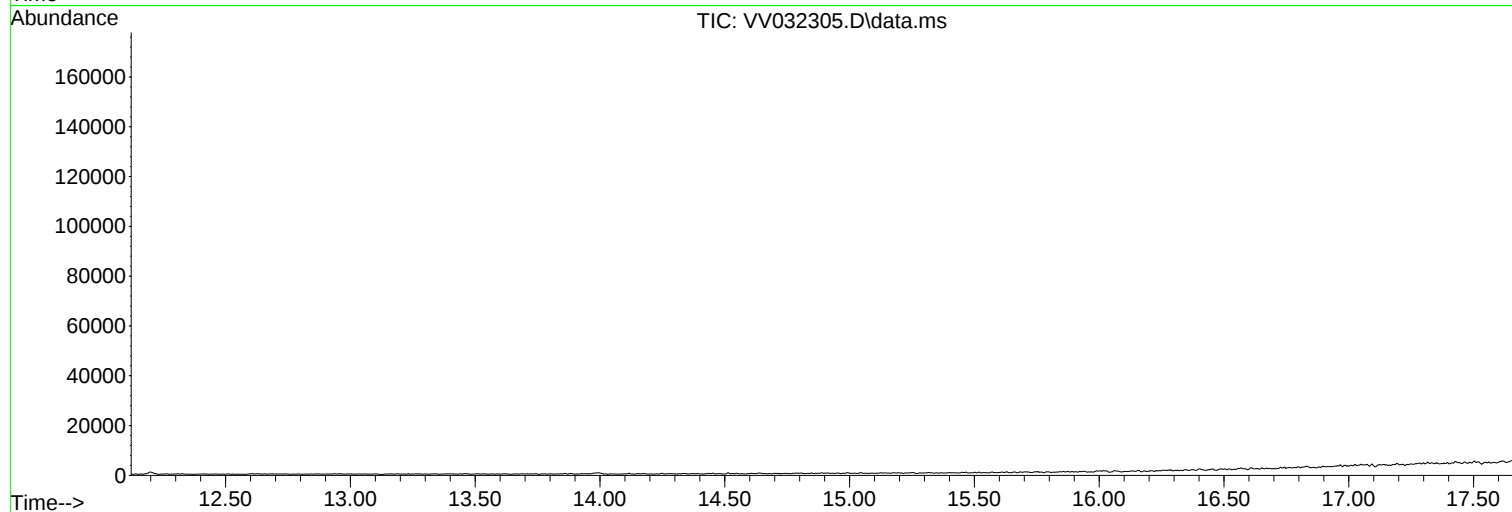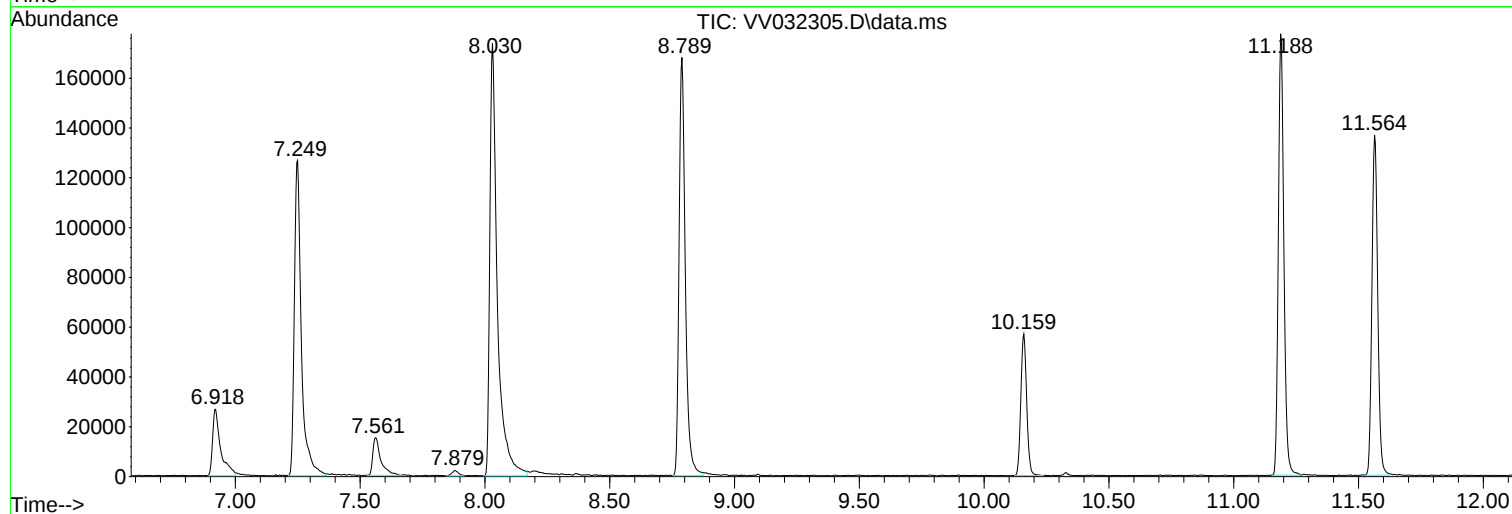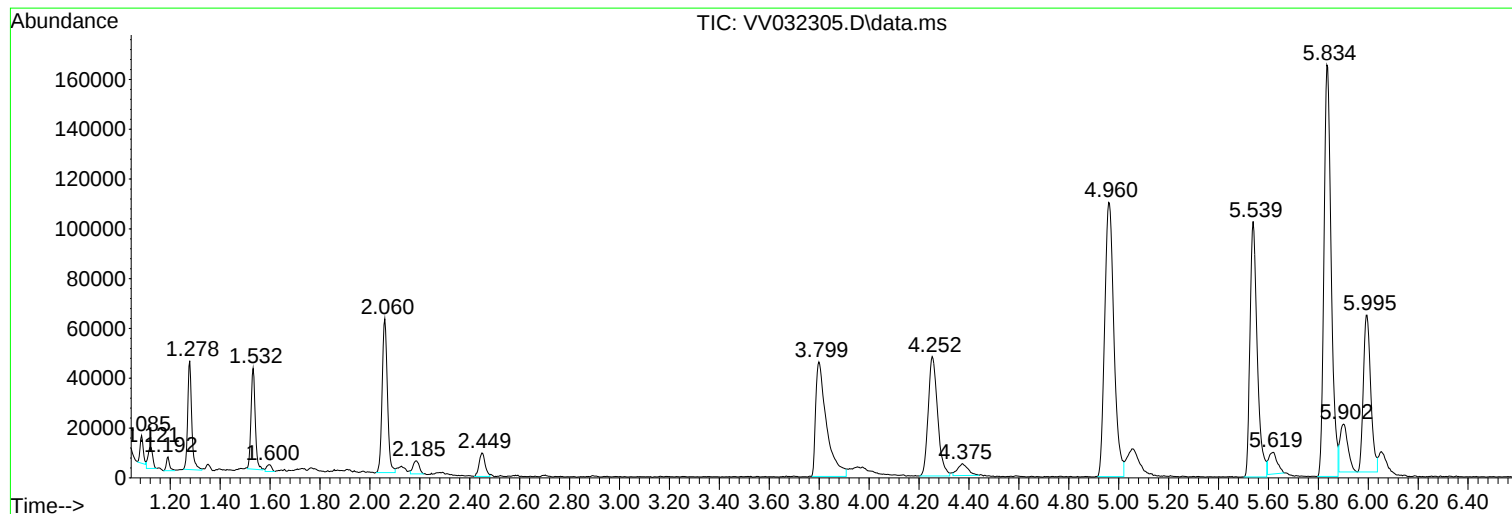

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100623\
Data File : VV032305.D
Acq On : 06 Oct 2023 16:42
Operator : SY/MD
Sample : 04748-26DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX864DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100623\
Data File : VV032305.D
Acq On : 06 Oct 2023 16:42
Operator : SY/MD
Sample : 04748-26DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX864DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc