

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100623\
 Data File : VV032310.D
 Acq On : 06 Oct 2023 18:45
 Operator : SY/MD
 Sample : 04774-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05K6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032310.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	18	24	33	rVB	9016	13217	2.90%	0.388%
2	1.278	67	74	90	rVB	40523	45254	9.92%	1.328%
3	1.532	145	153	166	rBV	40944	48327	10.60%	1.419%
4	2.060	306	317	331	rBV	64213	93682	20.54%	2.750%
5	2.182	349	355	366	rVB3	5669	9692	2.13%	0.284%
6	3.809	850	861	897	rBV	42535	146286	32.08%	4.294%
7	4.275	983	1006	1028	rBV3	140884	456054	100.00%	13.386%
8	4.960	1205	1219	1239	rBV2	118367	304482	66.76%	8.937%
9	5.053	1240	1248	1273	rVB2	10600	31108	6.82%	0.913%
10	5.539	1386	1399	1415	rBV	101401	213023	46.71%	6.253%
11	5.992	1527	1540	1554	rBV2	68887	145423	31.89%	4.268%
12	6.436	1666	1678	1691	rBV	81709	162403	35.61%	4.767%
13	6.918	1816	1828	1854	rBV2	30086	66035	14.48%	1.938%
14	7.249	1919	1931	1966	rBV	132282	258680	56.72%	7.593%
15	7.561	2019	2028	2055	rBV2	17237	38424	8.43%	1.128%
16	8.030	2164	2174	2210	rBV	184210	392433	86.05%	11.519%
17	8.182	2211	2221	2241	rVB	33238	63072	13.83%	1.851%
18	8.789	2399	2410	2429	rBV	169591	297022	65.13%	8.718%
19	10.159	2825	2836	2860	rBV	60776	98932	21.69%	2.904%
20	10.333	2879	2890	2901	rVB5	2957	4998	1.10%	0.147%
21	11.188	3145	3156	3178	rBV	180044	281392	61.70%	8.259%
22	11.564	3263	3273	3297	rVB	147684	236953	51.96%	6.955%




Sum of corrected areas: 3406892

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100623\
Data File : VV032310.D
Acq On : 06 Oct 2023 18:45
Operator : SY/MD
Sample : 04774-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

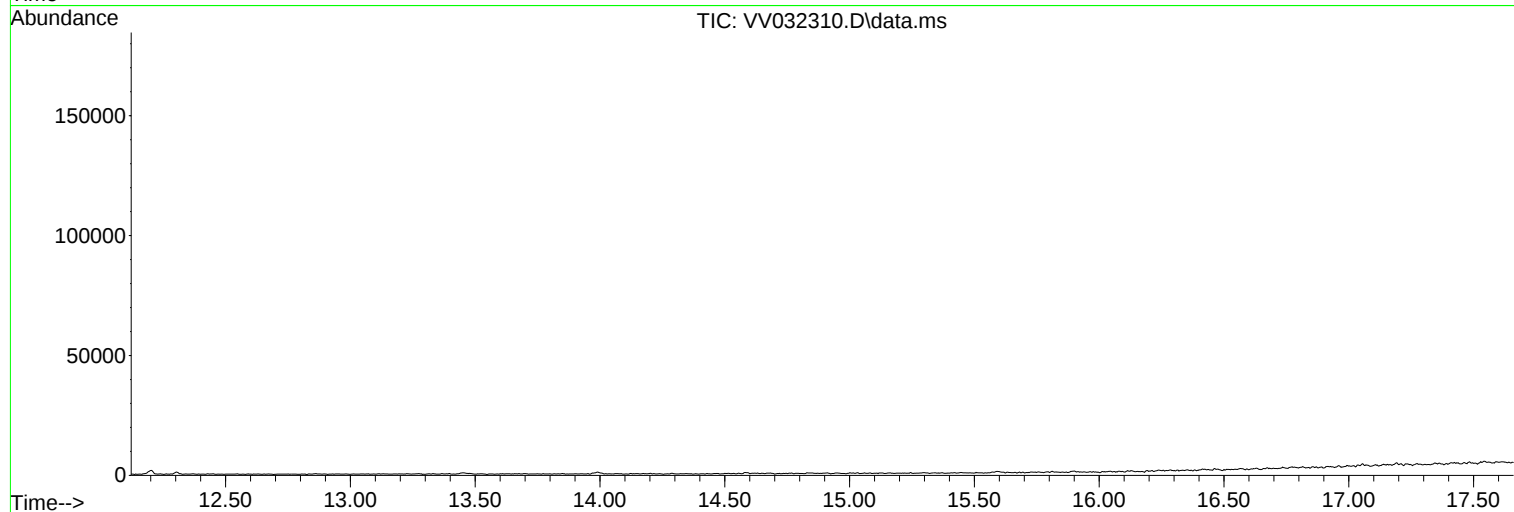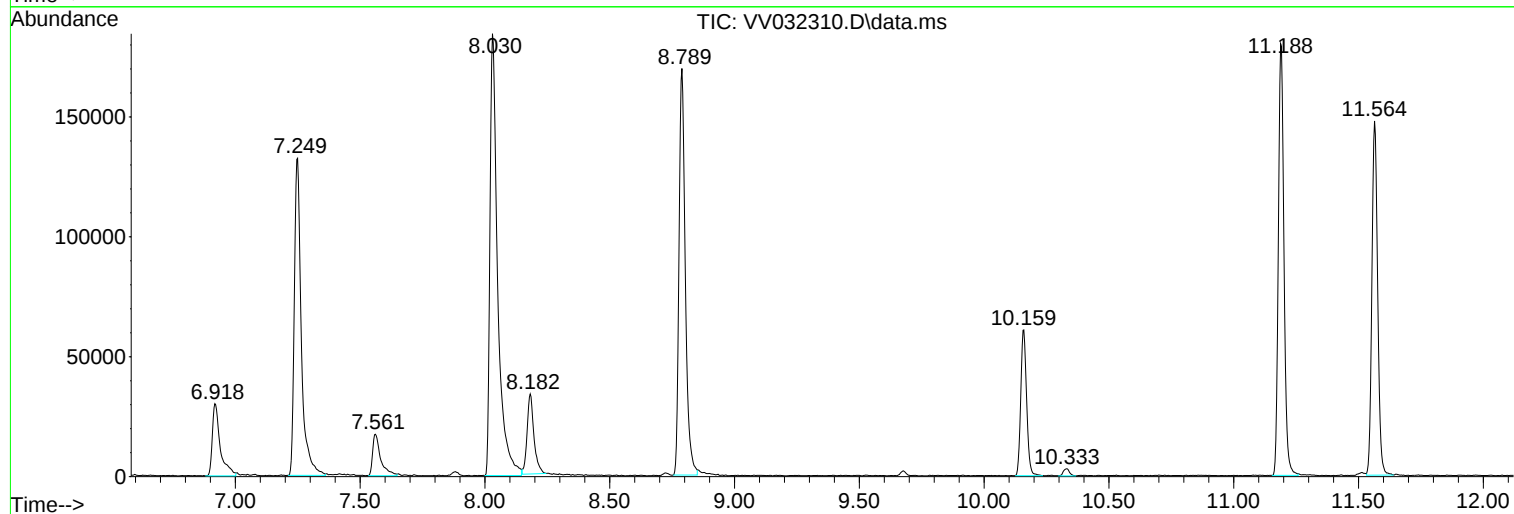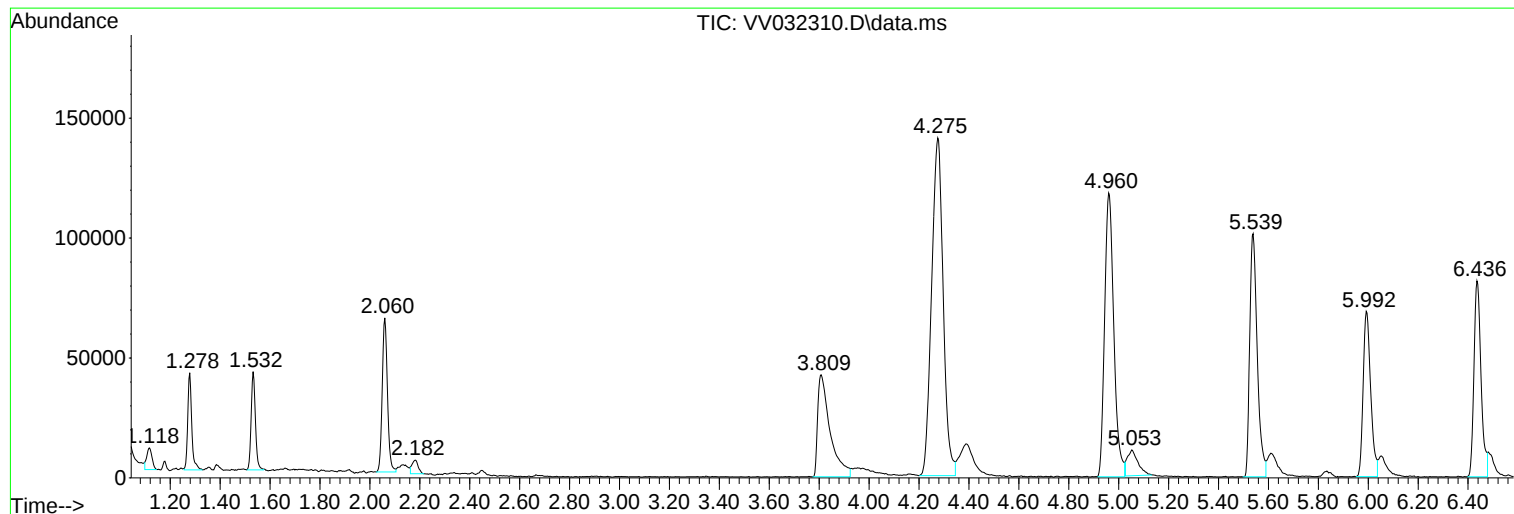

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100623\
Data File : VV032310.D
Acq On : 06 Oct 2023 18:45
Operator : SY/MD
Sample : 04774-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100623\
Data File : VV032310.D
Acq On : 06 Oct 2023 18:45
Operator : SY/MD
Sample : 04774-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc