


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100623\
Data File : VV032290.D
Acq On : 06 Oct 2023 08:33
Operator : SY/MD
Sample : BFB216
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB216

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Oct 07 05:00:49 2023

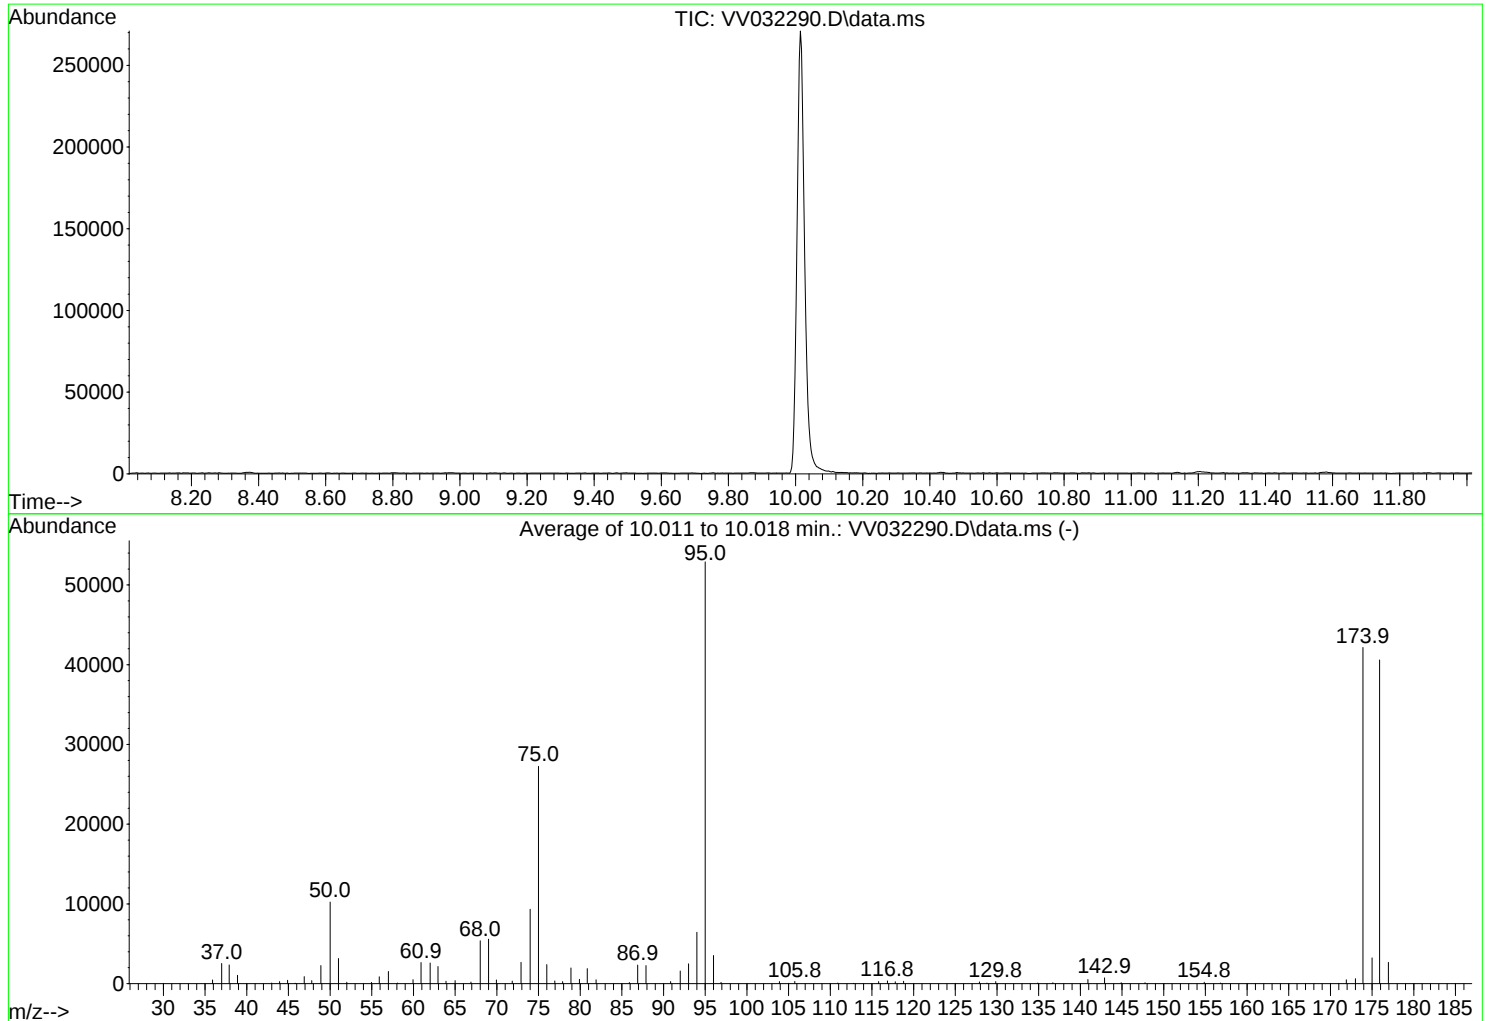

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	10229	PASS
75	95	30	80	51.5	27259	PASS
95	95	100	100	100.0	52901	PASS
96	95	5	9	6.7	3539	PASS
173	174	0.00	2	1.5	623	PASS
174	95	50	120	79.7	42157	PASS
175	174	5	9	7.6	3224	PASS
176	174	95	105	96.3	40589	PASS
177	176	5	10	6.6	2667	PASS

m/z	Abundance
40.10	172.0
43.90	369.0

Instrument :
MSVOA_V
ClientSampleId :
BFB216

m/z	Abundance
35.90	480.0
37.00	2561.0
37.90	2367.0
38.90	1055.0
40.00	171.0
44.00	614.0
44.90	435.0
46.90	857.0
47.80	391.0
48.90	2241.0
50.00	10030.0
51.00	3146.0
52.00	157.0
54.90	171.0
55.90	841.0
57.00	1422.0
58.10	108.0
60.00	500.0
60.90	2615.0
62.00	2538.0
63.00	2169.0
63.90	277.0
65.00	406.0
66.90	172.0
68.00	5323.0
69.00	5600.0
69.90	461.0
71.80	301.0
72.90	2532.0
74.00	9371.0
75.00	26680.0
76.00	2445.0
76.90	309.0
77.90	228.0
78.90	1922.0
79.90	509.0
80.80	1884.0
81.90	491.0
85.80	137.0
86.90	2304.0
87.90	2058.0
90.90	269.0
92.00	1540.0
93.00	2416.0
94.00	6202.0
95.00	51752.0
96.00	3714.0
96.90	139.0
103.90	247.0
105.70	299.0
110.90	100.0
115.80	235.0
116.80	311.0
117.80	241.0
118.80	296.0
127.90	205.0
128.80	115.0
129.90	228.0
136.70	116.0
140.90	462.0
142.90	668.0
144.90	110.0
147.80	139.0
154.90	177.0
156.80	113.0
171.00	101.0
171.90	444.0
173.00	555.0
173.90	39800.0
175.00	3015.0
175.90	38384.0
176.90	2501.0

Instrument :
MSVOA_V
ClientSampleId :
BFB216

m/z	Abundance
35.90	474.0
37.00	2646.0
37.90	2428.0
38.90	1095.0
39.90	159.0
43.00	106.0
44.00	649.0
44.90	427.0
45.80	100.0
46.90	916.0
47.80	393.0
48.90	2351.0
50.00	10623.0
51.00	3230.0
52.00	180.0
55.00	157.0
55.90	891.0
57.00	1588.0
58.10	110.0
60.00	513.0
60.90	2757.0
62.00	2706.0
63.00	2247.0
63.90	313.0
65.00	393.0
66.90	193.0
68.00	5518.0
69.00	5792.0
70.00	499.0
71.90	315.0
72.90	2764.0
74.00	9620.0
75.00	28304.0
76.00	2427.0
76.90	341.0
77.90	289.0
78.90	2053.0
79.90	552.0
80.90	1941.0
81.90	486.0
85.90	144.0
86.90	2444.0
87.90	2351.0
90.80	273.0
92.00	1643.0
93.00	2581.0
94.00	6697.0
95.00	55000.0
96.00	3602.0
96.90	164.0
103.90	276.0
105.80	286.0
110.90	122.0
115.80	259.0
116.80	340.0
117.80	255.0
118.80	313.0
127.90	240.0
128.80	102.0
129.90	267.0
134.90	109.0
136.70	135.0
140.90	523.0
142.90	737.0
144.90	140.0
147.70	146.0
154.80	212.0
156.80	129.0
171.90	496.0
173.00	626.0
173.90	43672.0
175.00	3322.0
175.90	42064.0
177.00	2780.0

Instrument :
MSVOA_V
ClientSampleId :
BFB216

m/z	Abundance
35.90	435.0
37.00	2402.0
37.90	2267.0
38.90	988.0
39.90	171.0
43.00	120.0
44.00	613.0
44.90	428.0
45.80	110.0
46.90	883.0
47.80	373.0
48.90	2189.0
50.00	10034.0
51.00	3054.0
52.00	191.0
55.00	150.0
55.90	868.0
57.00	1545.0
59.90	498.0
60.90	2558.0
62.00	2519.0
62.90	2040.0
63.90	318.0
65.00	337.0
66.90	211.0
68.00	5300.0
69.00	5367.0
70.00	434.0
71.90	329.0
72.90	2683.0
74.00	8985.0
75.00	26792.0
76.00	2287.0
77.00	383.0
77.90	292.0
78.90	1913.0
79.90	549.0
80.90	1816.0
81.90	449.0
86.00	132.0
86.90	2267.0
87.90	2411.0
90.80	272.0
92.00	1596.0
93.00	2473.0
94.00	6435.0
95.00	51952.0
96.00	3302.0
96.90	154.0
103.90	287.0
105.00	101.0
105.80	253.0
112.80	107.0
115.80	267.0
116.90	345.0
117.80	233.0
118.80	305.0
127.90	215.0
129.80	264.0
134.90	128.0
136.70	118.0
140.90	564.0
142.90	736.0
144.90	144.0
147.70	109.0
154.80	175.0
171.90	483.0
173.00	687.0
173.90	43000.0
175.00	3334.0
175.90	41320.0
177.00	2719.0

Instrument :
MSVOA_V
ClientSampleId :
BFB216