

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV100625\  
 Data File : VV039266.D  
 Acq On : 06 Oct 2025 12:13  
 Operator : SY/MD  
 Sample : VV1006MBL01  
 Misc : 5.00g/10.0mL/100uL/5.0mL/MSVOA\_V/MEOH  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 VV1006MBL01

Quant Time: Oct 07 03:31:10 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\82V092225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Sep 24 08:08:08 2025  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc      | Units       | Dev(Min) |
|-------------------------------|--------|-------|----------|-----------|-------------|----------|
| -----                         |        |       |          |           |             |          |
| Internal Standards            |        |       |          |           |             |          |
| 1) Pentafluorobenzene         | 4.600  | 168   | 491791   | 50.000    | ug/l        | 0.00     |
| 34) 1,4-Difluorobenzene       | 5.532  | 114   | 1015770  | 50.000    | ug/l        | 0.00     |
| 63) Chlorobenzene-d5          | 8.776  | 117   | 966866   | 50.000    | ug/l        | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 11.175 | 152   | 445450   | 50.000    | ug/l        | 0.00     |
|                               |        |       |          |           |             |          |
| System Monitoring Compounds   |        |       |          |           |             |          |
| 33) 1,2-Dichloroethane-d4     | 4.940  | 65    | 421917   | 59.277    | ug/l        | 0.00     |
| Spiked Amount                 | 50.000 | Range | 81 - 118 | Recovery  | = 118.560%# |          |
| 35) Dibromofluoromethane      | 4.500  | 113   | 381093   | 46.668    | ug/l        | 0.00     |
| Spiked Amount                 | 50.000 | Range | 80 - 119 | Recovery  | = 93.340%   |          |
| 50) Toluene-d8                | 7.236  | 98    | 1216997  | 50.743    | ug/l        | 0.00     |
| Spiked Amount                 | 50.000 | Range | 89 - 112 | Recovery  | = 101.480%  |          |
| 62) 4-Bromofluorobenzene      | 10.001 | 95    | 397285   | 40.238    | ug/l        | 0.00     |
| Spiked Amount                 | 50.000 | Range | 85 - 114 | Recovery  | = 80.480%#  |          |
|                               |        |       |          |           |             |          |
| Target Compounds              |        |       |          |           |             | Qvalue   |
| 5) Bromomethane               | 1.506  | 94    | 2389     | 0.424     | ug/l        | 90       |
| 6) Chloroethane               | 1.526  | 64    | 627      | Below Cal | #           | 44       |
| 10) Methyl Iodide             | 2.211  | 142   | 6155     | 0.839     | ug/l        | 99       |
| 11) Tert butyl alcohol        | 2.580  | 59    | 599      | 0.398     | ug/l #      | 94       |
| 13) Acrolein                  | 2.014  | 56    | 246      | 0.942     | ug/l #      | 1        |
| 16) Acetone                   | 2.130  | 43    | 1438     | Below Cal | #           | 64       |
| 17) Carbon Disulfide          | 2.256  | 76    | 12571    | 0.554     | ug/l        | 99       |
| 20) Methylene Chloride        | 2.465  | 84    | 1595     | Below Cal | #           | 86       |
| 21) trans-1,2-Dichloroethene  | 2.709  | 96    | 1619     | 0.205     | ug/l #      | 72       |
| 31) Cyclohexane               | 4.596  | 56    | 9297     | 0.732     | ug/l #      | 1        |
| 36) 1,1-Dichloropropene       | 4.600  | 75    | 40484    | 3.279     | ug/l #      | 47       |
| 38) Carbon Tetrachloride      | 4.600  | 117   | 50517    | 3.348     | ug/l #      | 17       |
| 41) Methacrylonitrile         | 4.130  | 41    | 106      | 1.926     | ug/l #      | 31       |
| 49) 1,4-Dioxane               | 6.313  | 88    | 42       | 0.281     | ug/l #      | 1        |
| 58) 2-Chloroethyl Vinyl ether | 6.821  | 63    | 95       | 9.636     | ug/l #      | 47       |
| 59) 2-Hexanone                | 7.947  | 43    | 111      | 2.336     | ug/l        | 73       |
| 70) Styrene                   | 9.480  | 104   | 40       | 1.563     | ug/l #      | 22       |
| 76) 1,2,3-Trichloropropane    | 10.001 | 75    | 193604   | 19.089    | ug/l #      | 56       |
| 81) trans-1,4-Dichloro-2-b... | 10.001 | 75    | 193604   | 45.827    | ug/l #      | 13       |
| 87) 1,3-Dichlorobenzene       | 11.130 | 146   | 3463     | 0.204     | ug/l        | 92       |
| 92) 1,2-Dibromo-3-Chloropr... | 12.384 | 75    | 76       | Below Cal | #           | 5        |
| 93) 1,2,4-Trichlorobenzene    | 13.210 | 180   | 2868     | 0.316     | ug/l        | 93       |
| 94) Hexachlorobutadiene       | 13.371 | 225   | 2227     | 0.472     | ug/l        | 97       |
| 96) 1,2,3-Trichlorobenzene    | 13.680 | 180   | 3051     | 0.328     | ug/l        | 90       |
| -----                         |        |       |          |           |             |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV100625\  
Data File : VV039266.D  
Acq On : 06 Oct 2025 12:13  
Operator : SY/MD  
Sample : VV1006MBL01  
Misc : 5.00g/10.0mL/100uL/5.0mL/MSVOA\_V/MEOH  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
VV1006MBL01

Quant Time: Oct 07 03:31:10 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\82V092225W.M  
Quant Title : SW846 8260  
QLast Update : Wed Sep 24 08:08:08 2025  
Response via : Initial Calibration

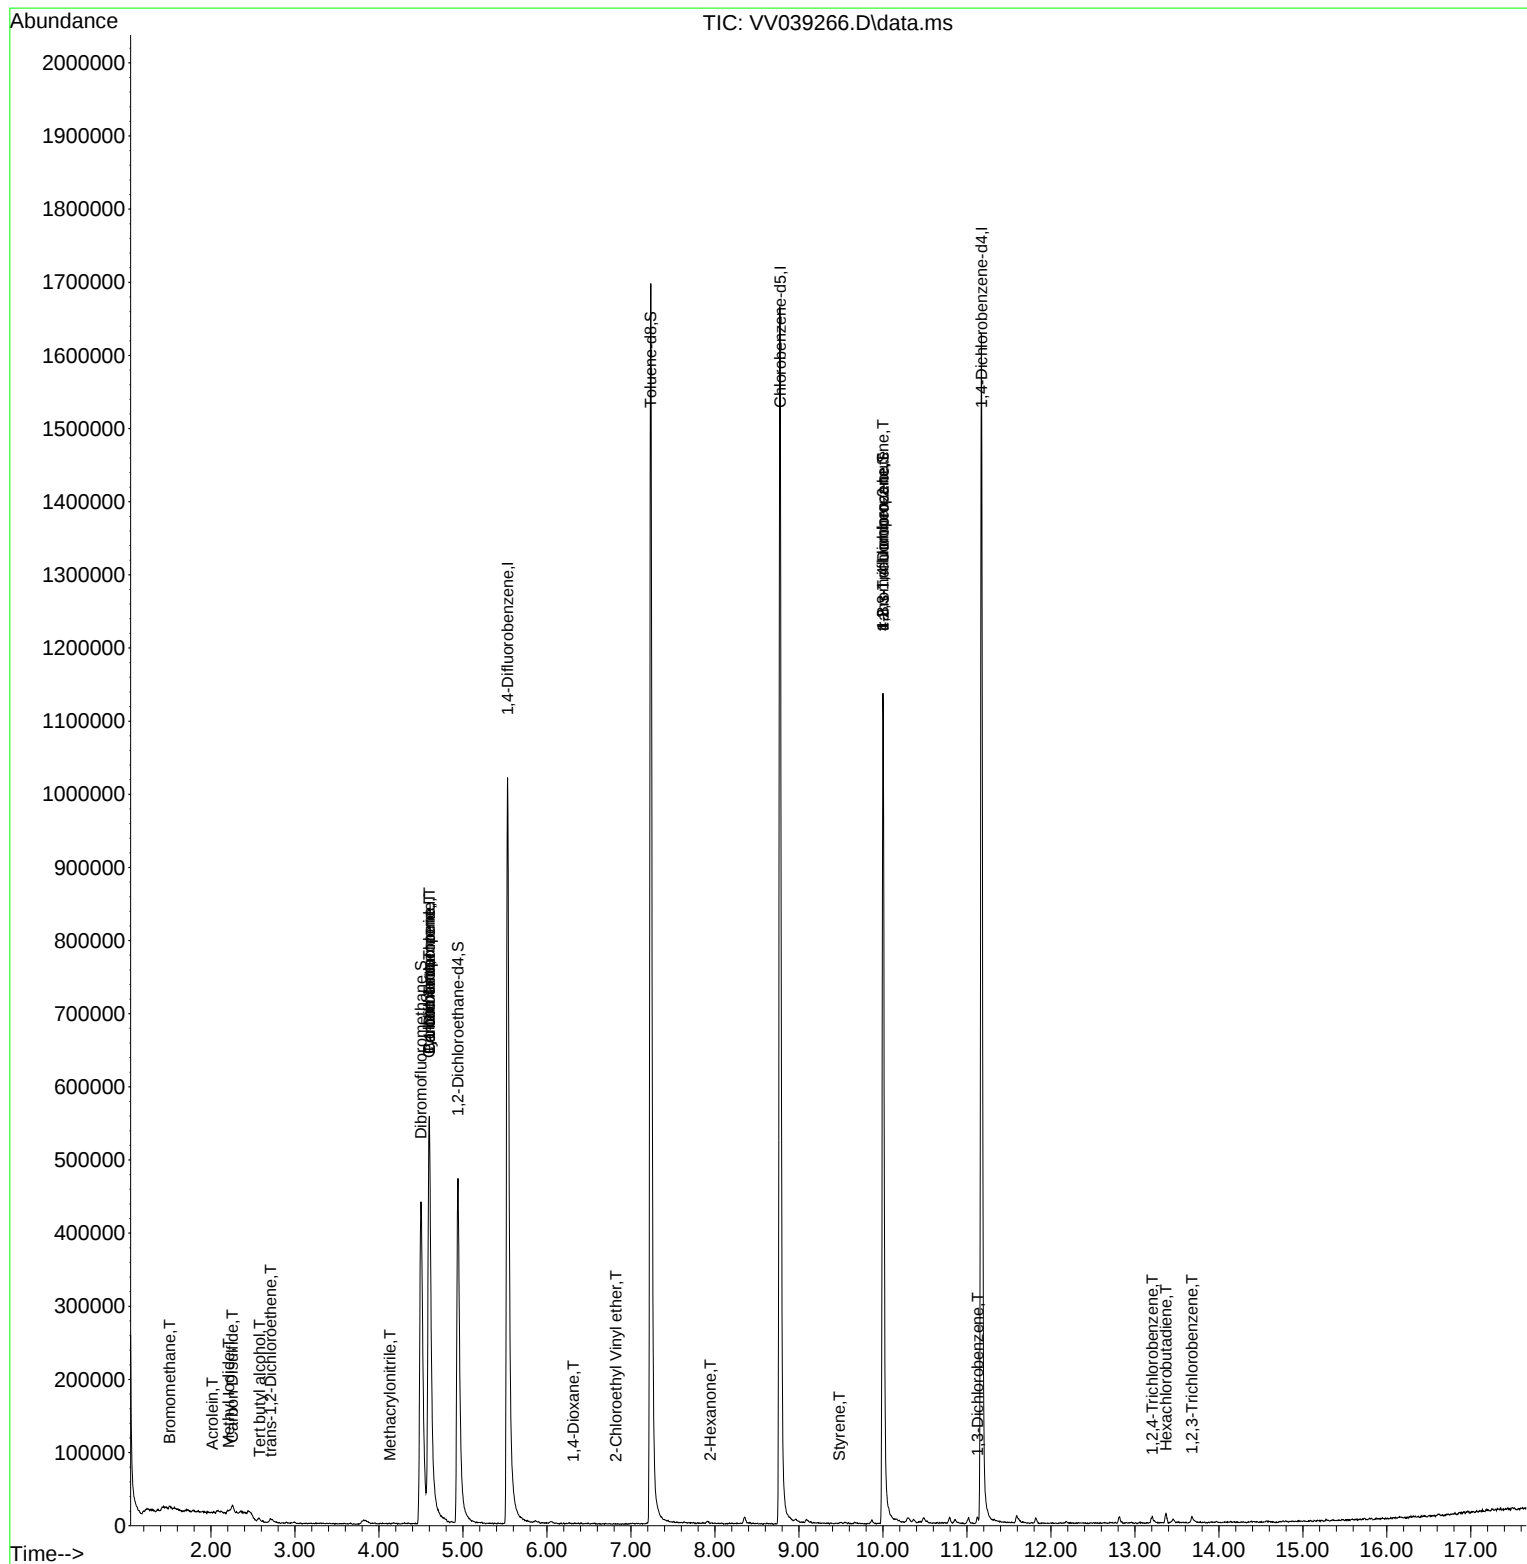



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.600 min Scan# 1106

Delta R.T. 0.003 min

Lab File: VV039266.D

Acq: 06 Oct 2025 12:13

Instrument :

MSVOA\_V

ClientSampleId :





VV1006MBL01

Tgt Ion:168 Resp: 491791

Ion Ratio Lower Upper

168 100

99 59.1 49.6 74.4

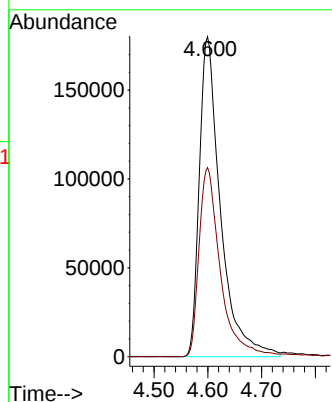

#5

Bromomethane

Concen: 0.424 ug/l

RT: 1.506 min Scan# 145

Delta R.T. 0.012 min

Lab File: VV039266.D




Acq: 06 Oct 2025 12:13


Tgt Ion: 94 Resp: 2389

Ion Ratio Lower Upper

94 100

96 103.3 74.9 112.3


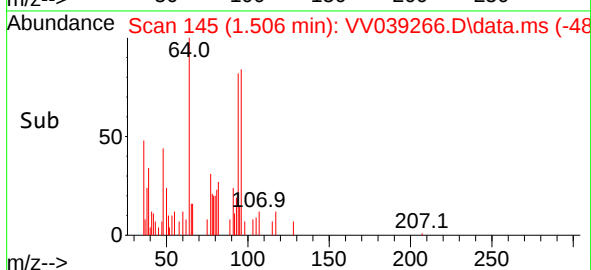
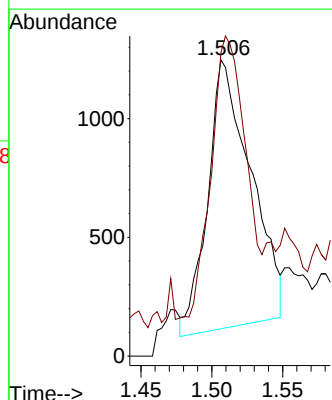





#6  
Chloroethane  
Concen: Below Cal  
RT: 1.526 min Scan# 11  
Delta R.T. -0.032 min  
Lab File: VV039266.D  
Acq: 06 Oct 2025 12:13




Instrument :  
MSVOA\_V  
ClientSampleId :  
VV1006MBL01


Tgt Ion: 64 Resp: 627  
Ion Ratio Lower Upper  
64 100  
66 0.0 24.6 36.8#

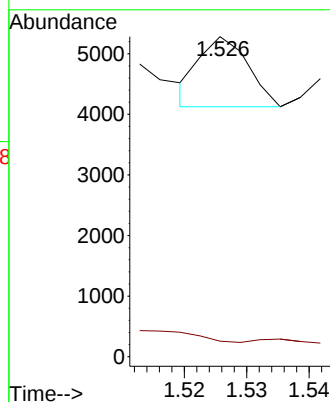

#10  
Methyl Iodide  
Concen: 0.839 ug/l  
RT: 2.211 min Scan# 364  
Delta R.T. 0.016 min  
Lab File: VV039266.D  
Acq: 06 Oct 2025 12:13

Tgt Ion:142 Resp: 6155  
Ion Ratio Lower Upper  
142 100  
127 44.6 36.3 54.5  
141 14.1 11.2 16.8


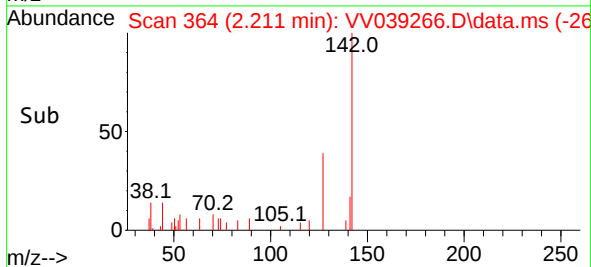
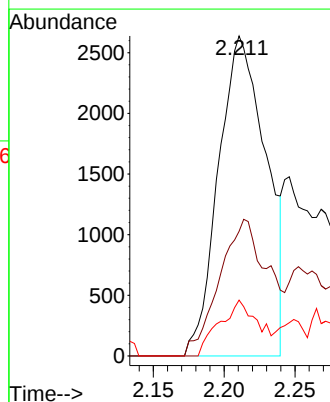
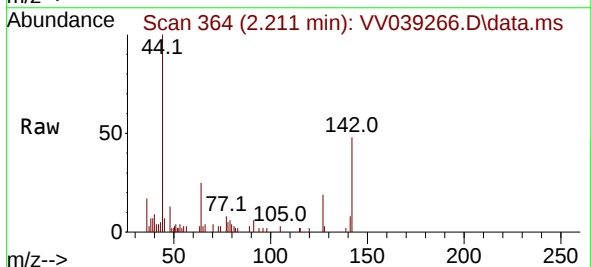




#11  
Tert butyl alcohol  
Concen: 0.398 ug/l  
RT: 2.580 min Scan# 41  
Delta R.T. 0.016 min  
Lab File: VV039266.D  
Acq: 06 Oct 2025 12:13




Instrument :  
MSVOA\_V  
ClientSampleId :  
VV1006MBL01


Tgt Ion: 59 Resp: 599  
Ion Ratio Lower Upper  
59 100  
57 11.9 7.8 11.8#

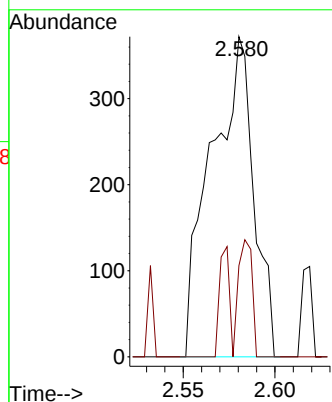

#13  
Acrolein  
Concen: 0.942 ug/l  
RT: 2.014 min Scan# 303  
Delta R.T. 0.006 min  
Lab File: VV039266.D  
Acq: 06 Oct 2025 12:13

Tgt Ion: 56 Resp: 246  
Ion Ratio Lower Upper  
56 100  
55 155.7 56.2 84.4#


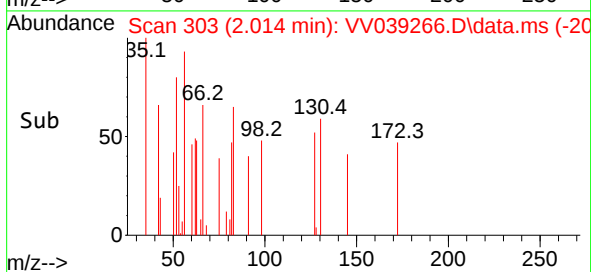
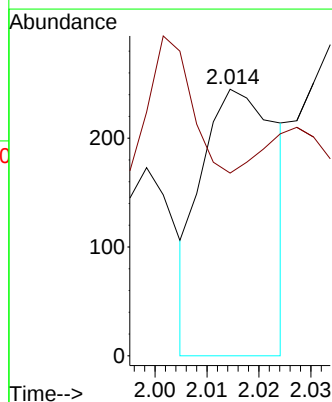





#16  
Acetone  
Concen: Below Cal  
RT: 2.130 min Scan# 31  
Delta R.T. 0.012 min  
Lab File: VV039266.D  
Acq: 06 Oct 2025 12:13




Instrument :  
MSVOA\_V  
ClientSampleId :  
VV1006MBL01


Tgt Ion: 43 Resp: 1438  
Ion Ratio Lower Upper  
43 100  
58 52.5 25.8 38.6#

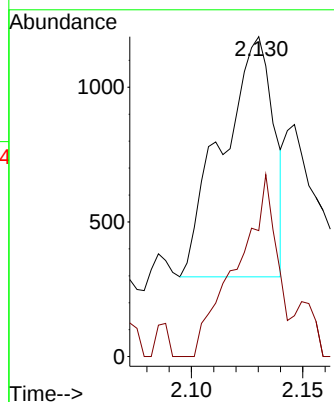

#17  
Carbon Disulfide  
Concen: 0.554 ug/l  
RT: 2.256 min Scan# 378  
Delta R.T. 0.003 min  
Lab File: VV039266.D  
Acq: 06 Oct 2025 12:13

Tgt Ion: 76 Resp: 12571  
Ion Ratio Lower Upper  
76 100  
78 9.5 7.4 11.0


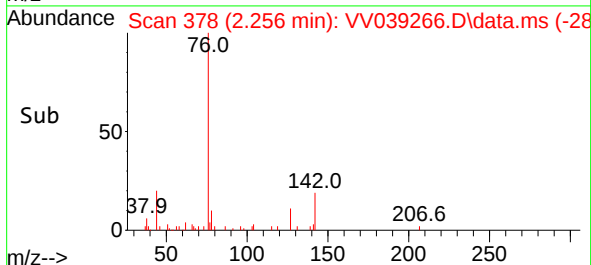
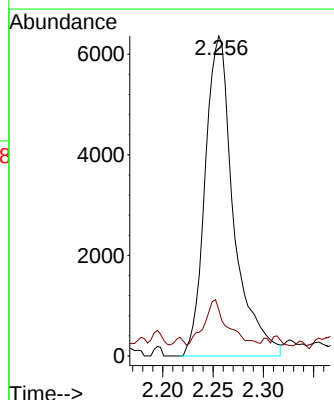
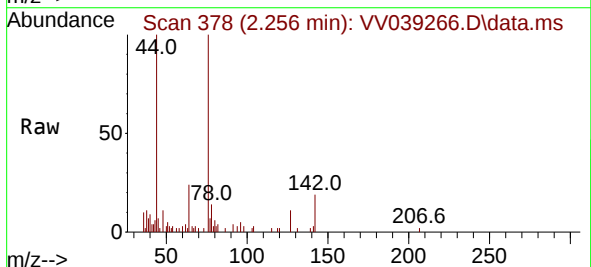




#20  
Methylene Chloride  
Concen: Below Cal  
RT: 2.465 min Scan# 440  
Delta R.T. 0.010 min  
Lab File: VV039266.D  
Acq: 06 Oct 2025 12:13




Instrument :  
MSVOA\_V  
ClientSampleId :  
VV1006MBL01


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 84    | Resp: | 1595  |
| Ion      | Ratio | Lower | Upper |
| 84       | 100   |       |       |
| 49       | 119.7 | 102.8 | 154.2 |
| 51       | 70.2  | 31.9  | 47.9# |
| 86       | 67.2  | 51.2  | 76.8  |

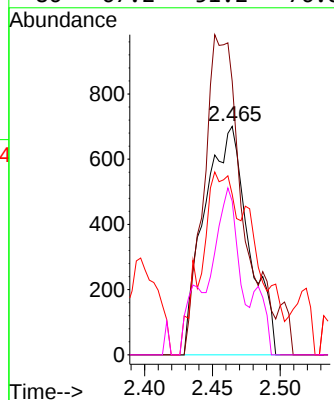

#21  
trans-1,2-Dichloroethene  
Concen: 0.205 ug/l  
RT: 2.709 min Scan# 519  
Delta R.T. 0.009 min  
Lab File: VV039266.D  
Acq: 06 Oct 2025 12:13

|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 96    | Resp: | 1619   |
| Ion      | Ratio | Lower | Upper  |
| 96       | 100   |       |        |
| 61       | 98.9  | 112.8 | 169.2# |
| 98       | 53.2  | 51.1  | 76.7   |


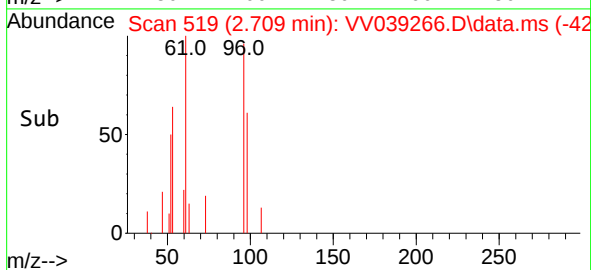
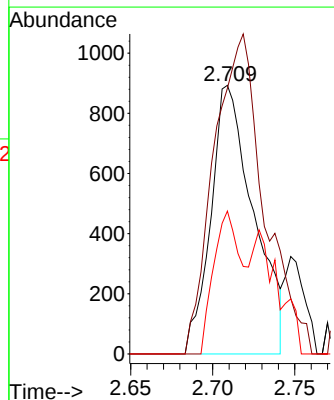





#31  
Cyclohexane  
Concen: 0.732 ug/l  
RT: 4.596 min Scan# 1106  
Delta R.T. 0.016 min  
Lab File: VV039266.D  
Acq: 06 Oct 2025 12:13




Instrument :  
MSVOA\_V  
ClientSampleId :  
VV1006MBL01


Tgt Ion: 56 Resp: 9297  
Ion Ratio Lower Upper  
56 100  
69 190.1 26.2 39.2#  
84 122.1 70.3 105.5#

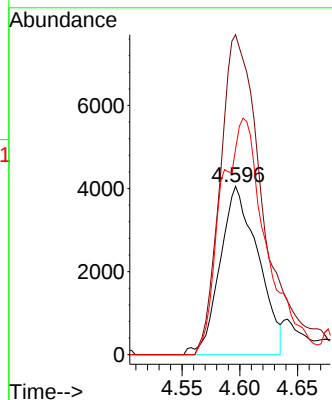

#33  
1,2-Dichloroethane-d4  
Concen: 59.277 ug/l  
RT: 4.940 min Scan# 1213  
Delta R.T. 0.003 min  
Lab File: VV039266.D  
Acq: 06 Oct 2025 12:13

Tgt Ion: 65 Resp: 421917  
Ion Ratio Lower Upper  
65 100  
67 53.1 0.0 107.0

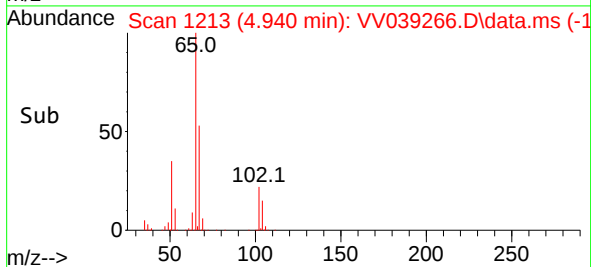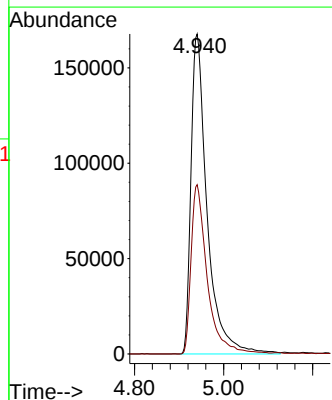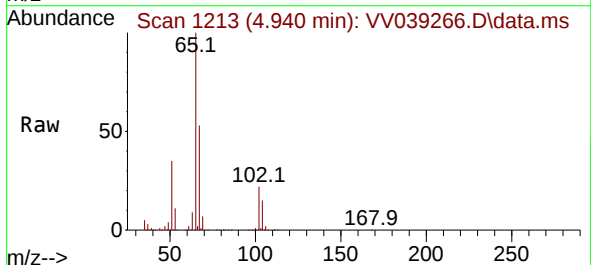



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 5.532 min Scan# 1

Delta R.T. 0.003 min

Lab File: VV039266.D

Acq: 06 Oct 2025 12:13

Instrument :

MSVOA\_V

ClientSampleId :

VV1006MBL01





Tgt Ion:114 Resp: 1015770

Ion Ratio Lower Upper

114 100

63 19.4 0.0 42.6

88 15.4 0.0 30.8

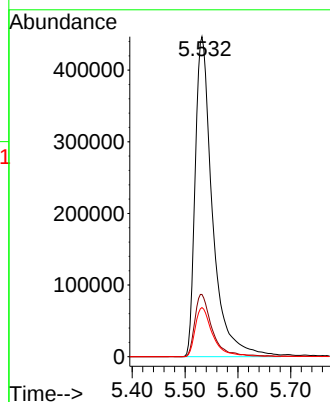

#35

Dibromofluoromethane

Concen: 46.668 ug/l

RT: 4.500 min Scan# 1076

Delta R.T. 0.003 min

Lab File: VV039266.D

Acq: 06 Oct 2025 12:13




Tgt Ion:113 Resp: 381093


Ion Ratio Lower Upper

113 100

111 101.8 82.4 123.6

192 17.8 13.8 20.8

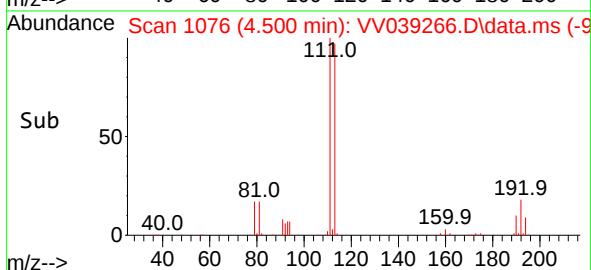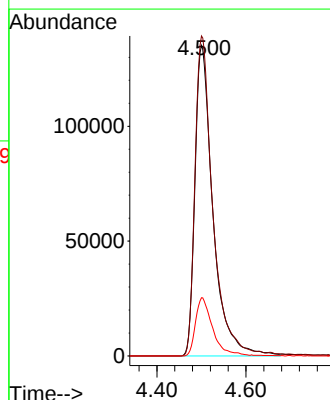



#36

1,1-Dichloropropene

Concen: 3.279 ug/l

RT: 4.600 min Scan# 1107

Delta R.T. -0.141 min

Lab File: VV039266.D

Acq: 06 Oct 2025 12:13

Instrument :

MSVOA\_V

ClientSampleId :

VV1006MBL01





Tgt Ion: 75 Resp: 40484

Ion Ratio Lower Upper

75 100

110 6.1 18.1 54.1#

77 0.2 24.8 37.2#

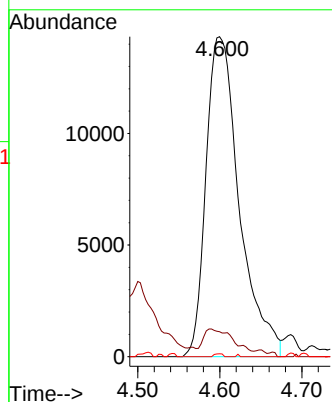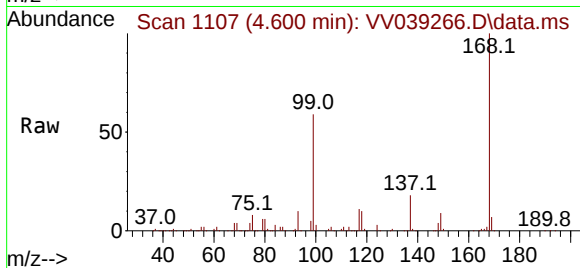

#38

Carbon Tetrachloride

Concen: 3.348 ug/l

RT: 4.600 min Scan# 1107

Delta R.T. -0.132 min

Lab File: VV039266.D

Acq: 06 Oct 2025 12:13




Tgt Ion: 117 Resp: 50517


Ion Ratio Lower Upper

117 100

119 6.2 77.2 115.8#

121 0.0 24.2 36.2#


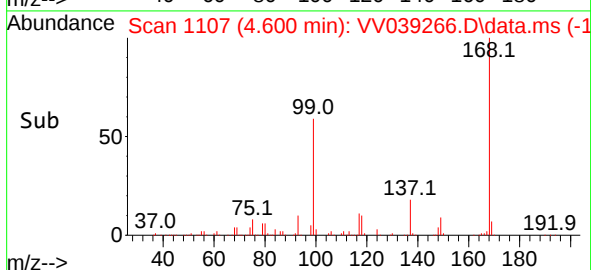
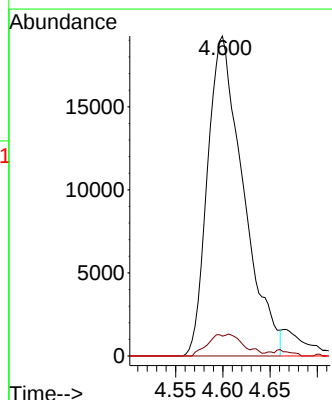
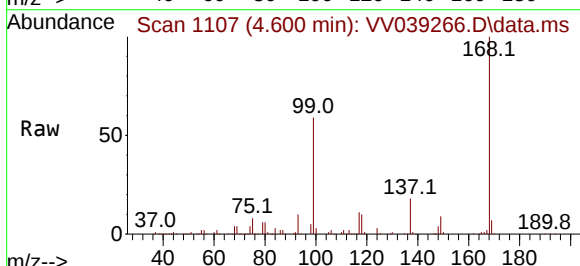




#41  
Methacrylonitrile  
Concen: 1.926 ug/l  
RT: 4.130 min Scan# 90  
Delta R.T. -0.023 min  
Lab File: VV039266.D  
Acq: 06 Oct 2025 12:13




Instrument :  
MSVOA\_V  
ClientSampleId :  
VV1006MBL01


|             |       |             |
|-------------|-------|-------------|
| Tgt Ion: 41 | Resp: | 106         |
| Ion         | Ratio | Lower Upper |
| 41          | 100   |             |
| 39          | 101.9 | 42.2 63.2#  |
| 67          | 0.0   | 67.9 101.9# |
| 52          | 37.7  | 26.7 40.1   |

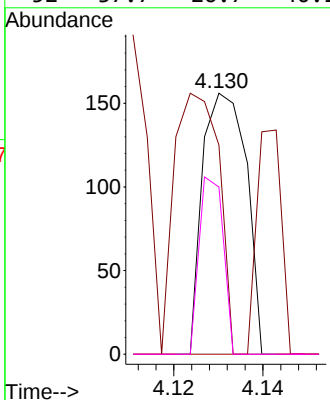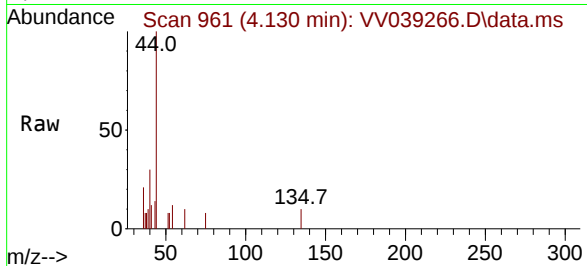

#49  
1,4-Dioxane  
Concen: 0.281 ug/l  
RT: 6.313 min Scan# 1640  
Delta R.T. 0.026 min  
Lab File: VV039266.D  
Acq: 06 Oct 2025 12:13

|             |       |             |
|-------------|-------|-------------|
| Tgt Ion: 88 | Resp: | 42          |
| Ion         | Ratio | Lower Upper |
| 88          | 100   |             |
| 43          | 285.7 | 25.1 37.7#  |
| 58          | 0.0   | 53.6 80.4#  |

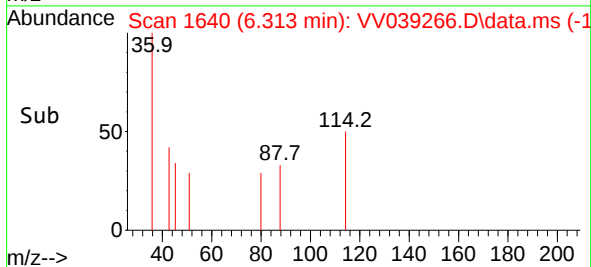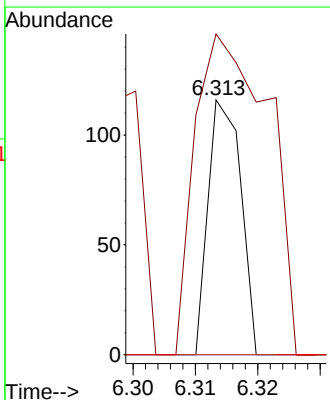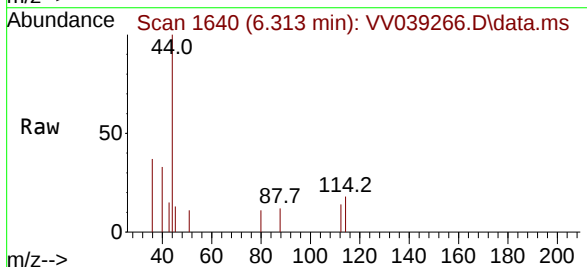

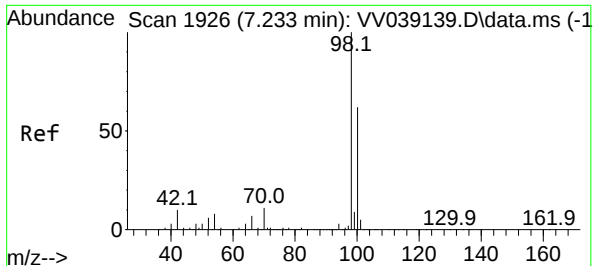

#50

Toluene-d8

Concen: 50.743 ug/l

RT: 7.236 min Scan# 1926

Delta R.T. 0.003 min

Lab File: VV039266.D

Acq: 06 Oct 2025 12:13

Instrument :

MSVOA\_V

ClientSampleId :





VV1006MBL01

Tgt Ion: 98 Resp: 1216997

Ion Ratio Lower Upper

98 100

100 64.5 52.2 78.2

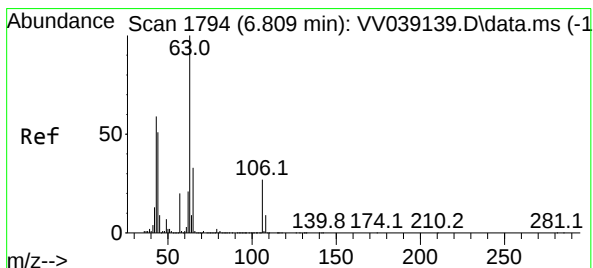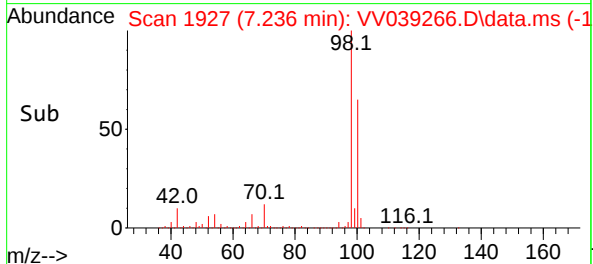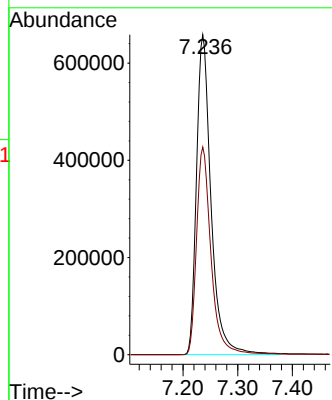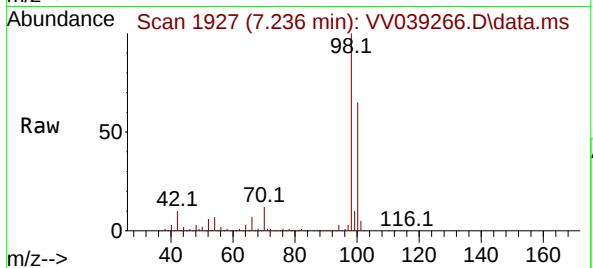

#58

2-Chloroethyl Vinyl ether

Concen: 9.636 ug/l

RT: 6.821 min Scan# 1798

Delta R.T. 0.012 min

Lab File: VV039266.D




Acq: 06 Oct 2025 12:13


Tgt Ion: 63 Resp: 95

Ion Ratio Lower Upper

63 100

106 0.0 22.1 33.1#

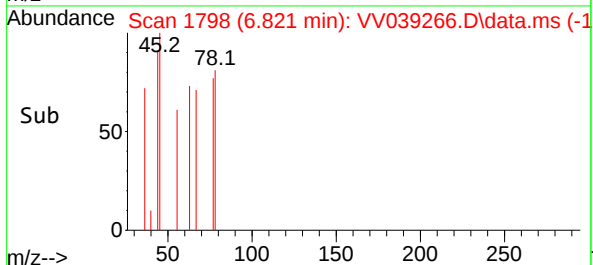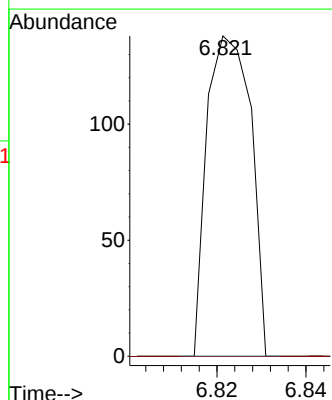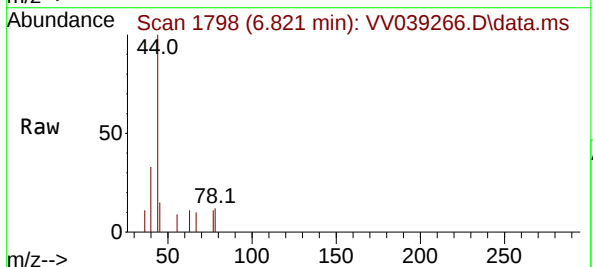



#59

2-Hexanone

Concen: 2.336 ug/l

RT: 7.947 min Scan# 2183

Delta R.T. -0.112 min

Lab File: VV039266.D

Acq: 06 Oct 2025 12:13

Instrument :

MSVOA\_V

ClientSampleId :





VV1006MBL01

Tgt Ion: 43 Resp: 111

Ion Ratio Lower Upper

43 100

58 36.9 28.3 85.0

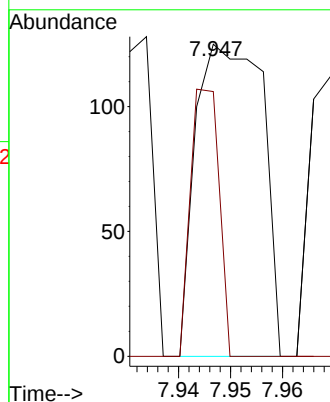

#62

4-Bromofluorobenzene

Concen: 40.238 ug/l

RT: 10.001 min Scan# 2787

Delta R.T. 0.003 min

Lab File: VV039266.D

Acq: 06 Oct 2025 12:13




Tgt Ion: 95 Resp: 397285


Ion Ratio Lower Upper

95 100

174 77.9 0.0 150.4

176 73.9 0.0 144.2


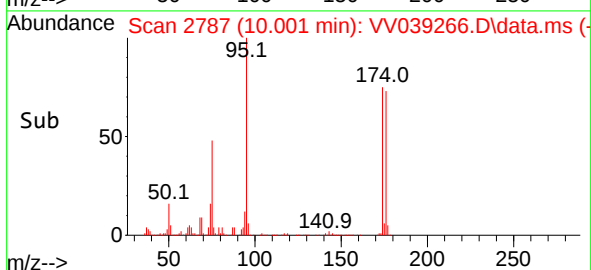
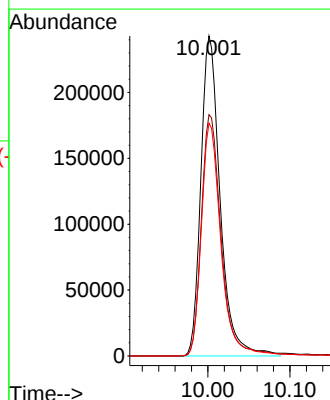





#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 8.776 min Scan# 2405  
Delta R.T. 0.003 min  
Lab File: VV039266.D  
Acq: 06 Oct 2025 12:13




Instrument :  
MSVOA\_V  
ClientSampleId :  
VV1006MBL01


Tgt Ion:117 Resp: 966866  
Ion Ratio Lower Upper  
117 100  
82 53.9 45.4 68.2  
119 31.4 25.6 38.4

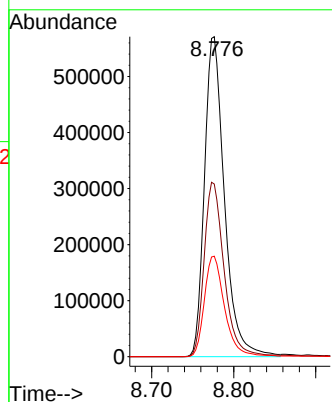

#70  
Styrene  
Concen: 1.563 ug/l  
RT: 9.480 min Scan# 2625  
Delta R.T. -0.004 min  
Lab File: VV039266.D  
Acq: 06 Oct 2025 12:13

Tgt Ion:104 Resp: 40  
Ion Ratio Lower Upper  
104 100  
78 105.0 39.8 59.6#  
103 0.0 43.4 65.2#


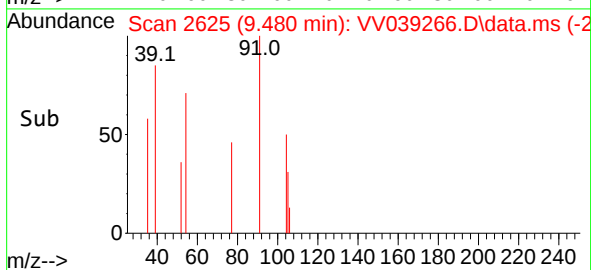
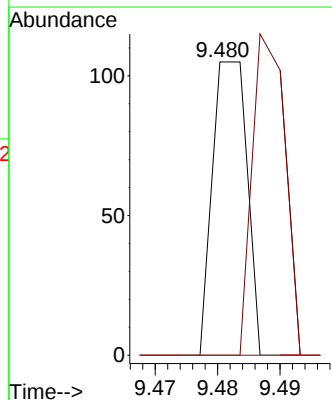



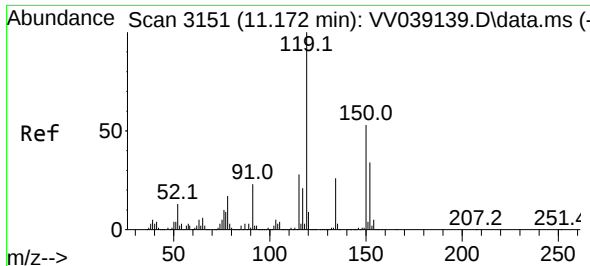

#72  
 1,4-Dichlorobenzene-d4  
 Concen: 50.000 ug/l  
 RT: 11.175 min Scan# 3151  
 Delta R.T. 0.003 min  
 Lab File: VV039266.D  
 Acq: 06 Oct 2025 12:13




Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 VV1006MBL01


Tgt Ion:152 Resp: 445450  
 Ion Ratio Lower Upper  
 152 100  
 115 60.4 44.8 134.4  
 150 154.7 0.0 353.8

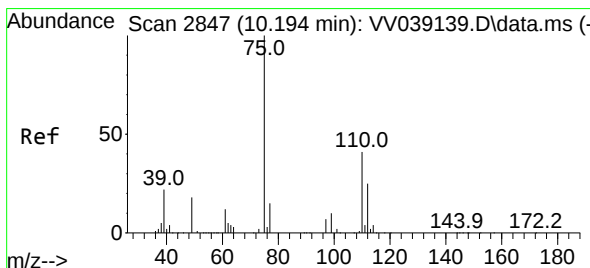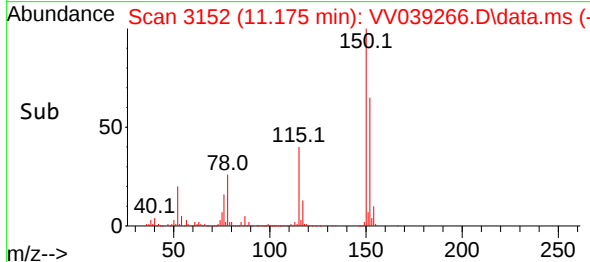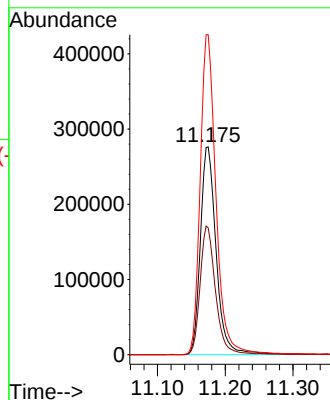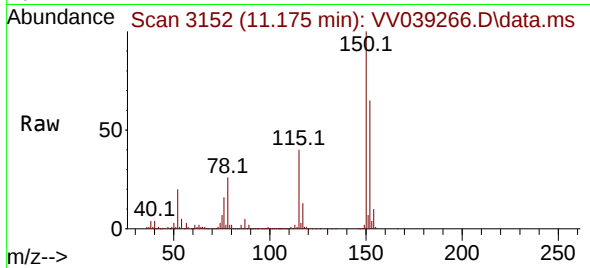

#76  
 1,2,3-Trichloropropane  
 Concen: 19.089 ug/l  
 RT: 10.001 min Scan# 2787  
 Delta R.T. -0.193 min  
 Lab File: VV039266.D  
 Acq: 06 Oct 2025 12:13

Tgt Ion: 75 Resp: 193604  
 Ion Ratio Lower Upper  
 75 100  
 77 1.4 11.3 33.8#


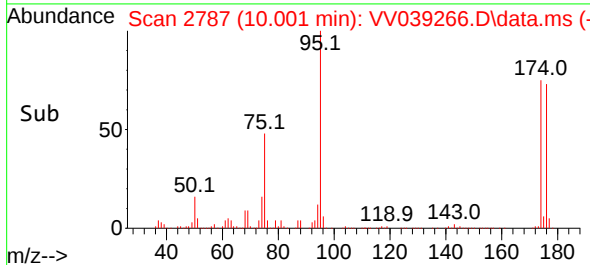
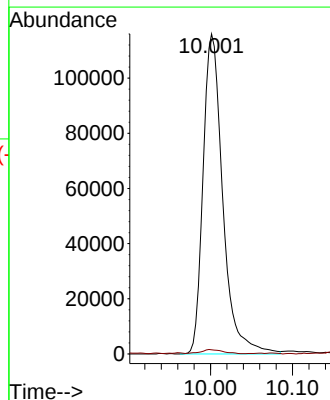
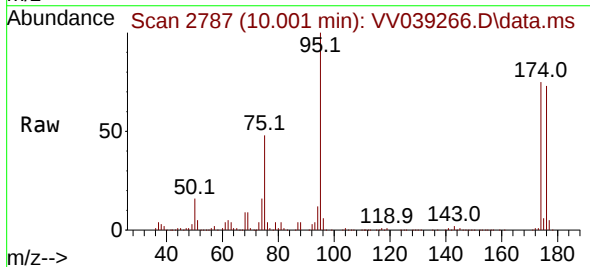




#81  
trans-1,4-Dichloro-2-butene  
Concen: 45.827 ug/l  
RT: 10.001 min Scan# 21  
Delta R.T. 0.074 min  
Lab File: VV039266.D  
Acq: 06 Oct 2025 12:13




Instrument :  
MSVOA\_V  
ClientSampleId :  
VV1006MBL01


Tgt Ion: 75 Resp: 193604  
Ion Ratio Lower Upper  
75 100  
53 0.4 72.5 108.7#  
89 0.0 37.2 55.8#

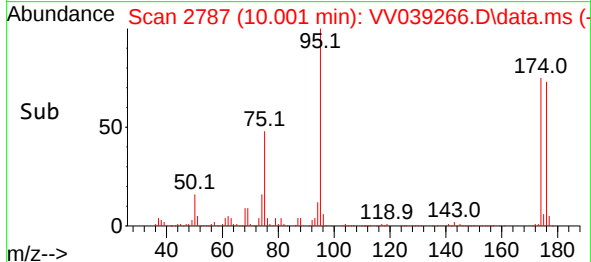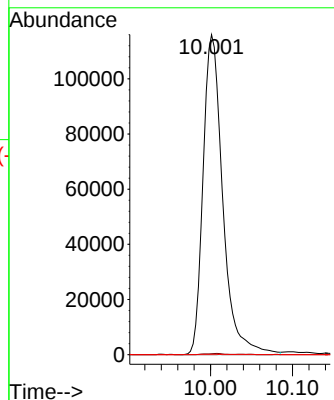

#87  
1,3-Dichlorobenzene  
Concen: 0.204 ug/l  
RT: 11.130 min Scan# 3138  
Delta R.T. 0.026 min  
Lab File: VV039266.D  
Acq: 06 Oct 2025 12:13

Tgt Ion: 146 Resp: 3463  
Ion Ratio Lower Upper  
146 100  
111 36.1 20.9 62.8  
148 69.6 31.8 95.3

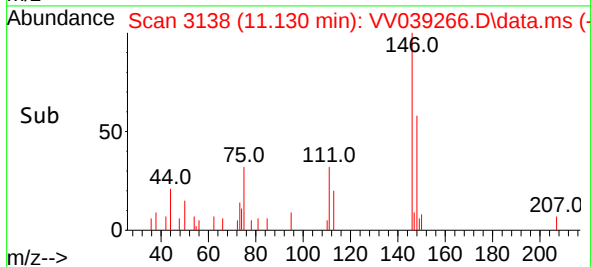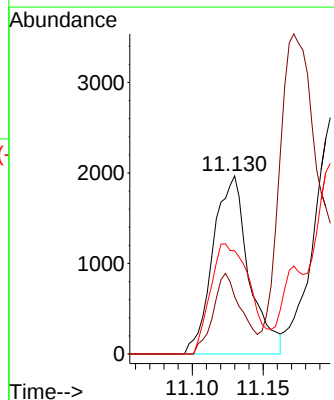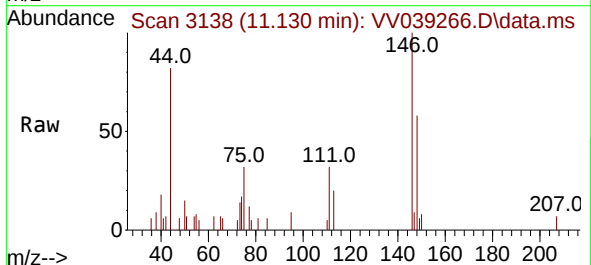



#92

1,2-Dibromo-3-Chloropropane

Concen: Below Cal

RT: 12.384 min Scan# 3

Delta R.T. 0.035 min

Lab File: VV039266.D

Acq: 06 Oct 2025 12:13

Instrument :

MSVOA\_V

ClientSampleId :

VV1006MBL01





Tgt Ion: 75 Resp: 76

Ion Ratio Lower Upper

75 100

155 0.0 38.6 115.8#

157 0.0 49.5 148.3#

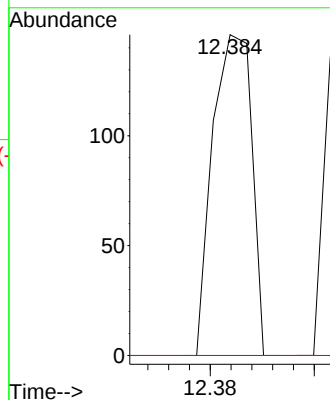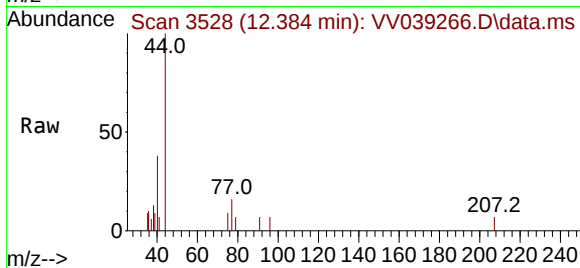

#93

1,2,4-Trichlorobenzene

Concen: 0.316 ug/l

RT: 13.210 min Scan# 3785

Delta R.T. 0.025 min

Lab File: VV039266.D

Acq: 06 Oct 2025 12:13




Tgt Ion: 180 Resp: 2868


Ion Ratio Lower Upper

180 100

182 102.6 47.1 141.4

145 30.5 16.3 48.8

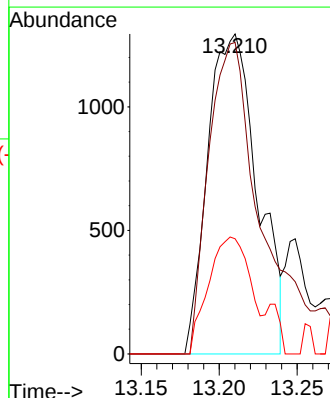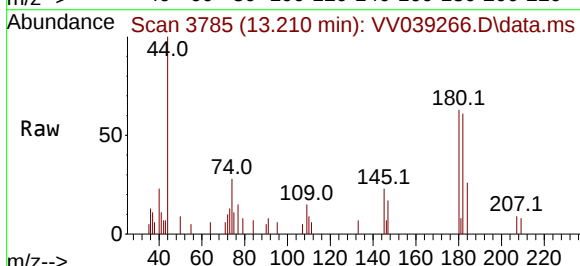



#94

Hexachlorobutadiene

Concen: 0.472 ug/l

RT: 13.371 min Scan# 3931

Delta R.T. 0.003 min

Lab File: VV039266.D

Acq: 06 Oct 2025 12:13

Instrument :

MSVOA\_V

ClientSampleId :

VV1006MBL01





Tgt Ion:225 Resp: 2227

Ion Ratio Lower Upper

225 100

223 65.5 31.6 94.7

227 60.7 31.8 95.4

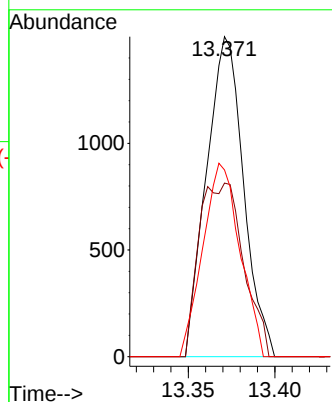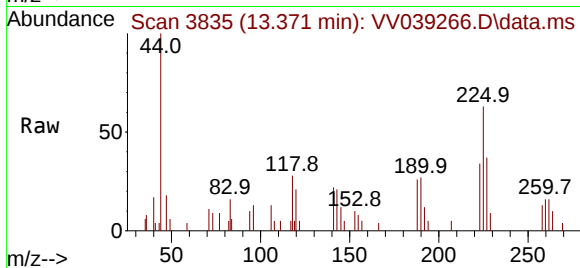

#96

1,2,3-Trichlorobenzene

Concen: 0.328 ug/l

RT: 13.680 min Scan# 3931

Delta R.T. 0.016 min

Lab File: VV039266.D

Acq: 06 Oct 2025 12:13

Tgt Ion:180 Resp: 3051

Ion Ratio Lower Upper

180 100

182 97.7 46.9 140.8

145 19.4 17.0 51.0

