
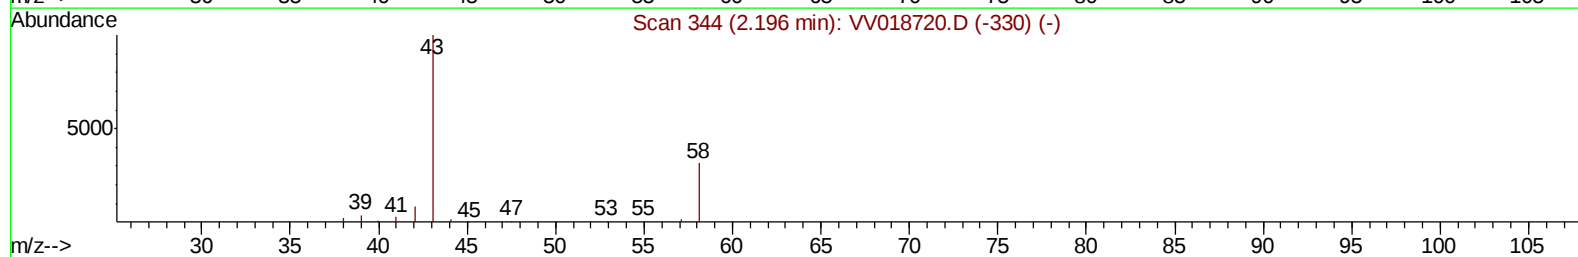
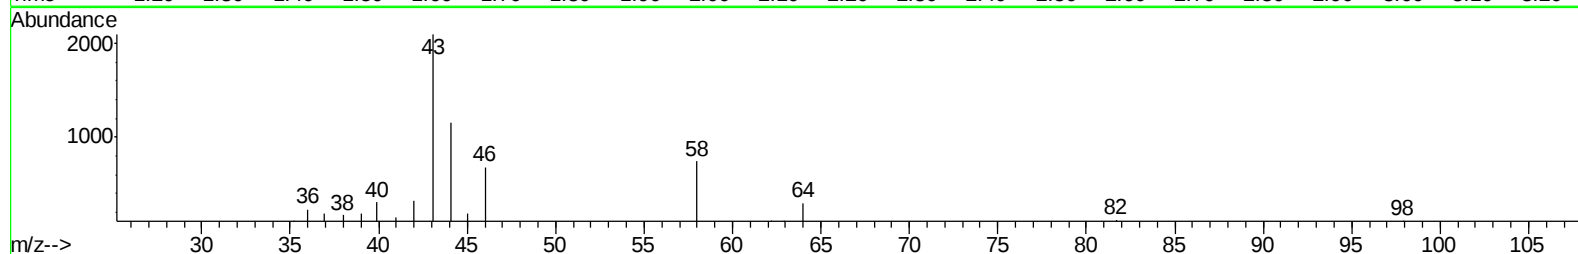


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100720\
Data File : VV018731.D
Acq On : 07 Oct 2020 15:36
Operator : SY/MD
Sample : L4284-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 38 Sample Multiplier: 1

Quant Time: Oct 08 02:54:57 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 08 02:46:20 2020
Response via : Initial Calibration

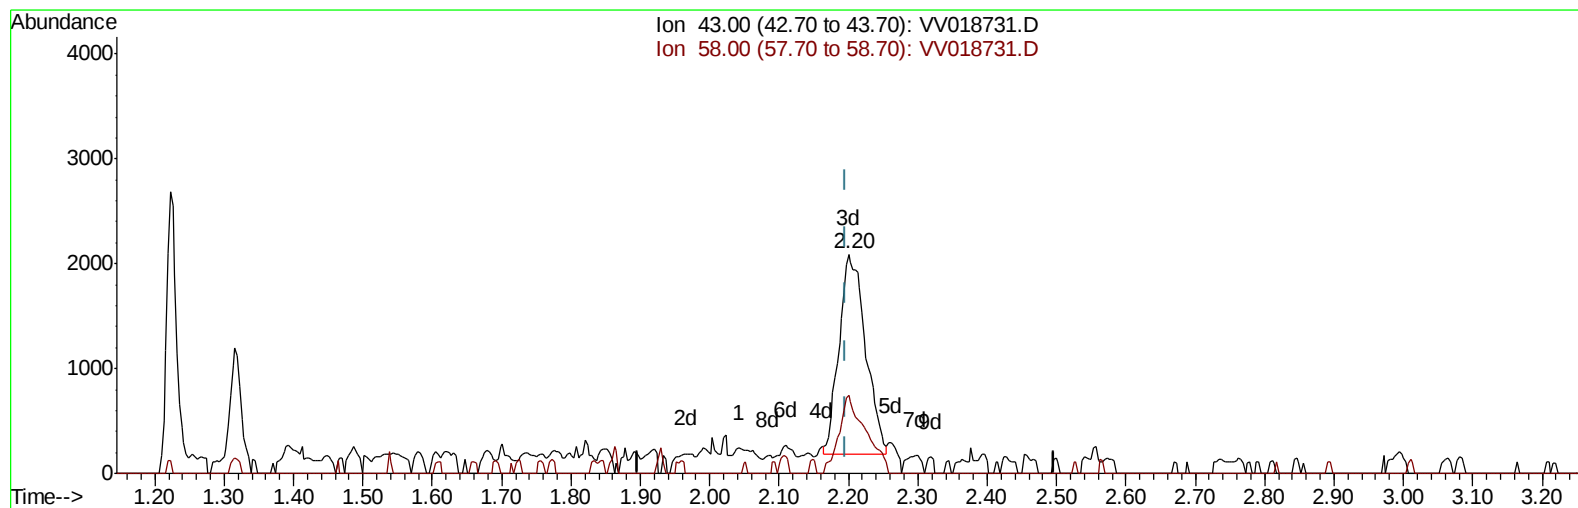

TIC: VV018731.D

(13) Acetone (T)

2.200min (+0.003) 6.13ug/L m

response 5057

Ion	Exp%	Act%
43.00	100	100
58.00	32.00	0.81
0.00	0.00	0.00
0.00	0.00	0.00