
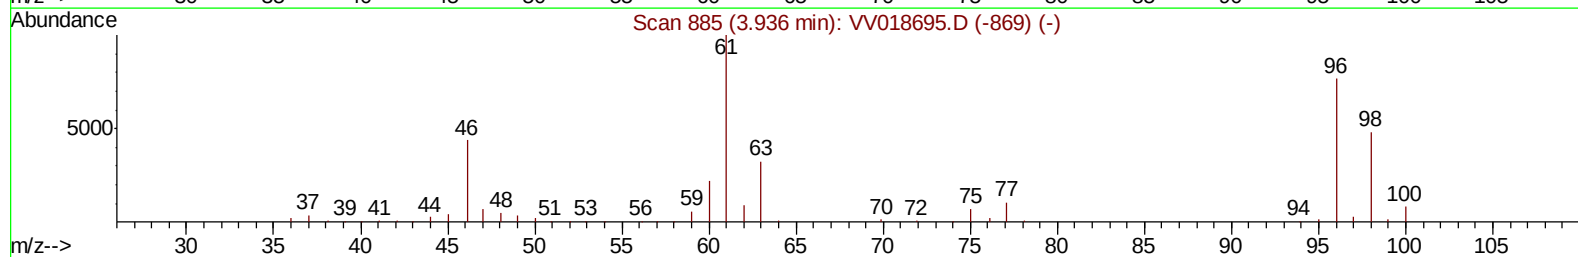
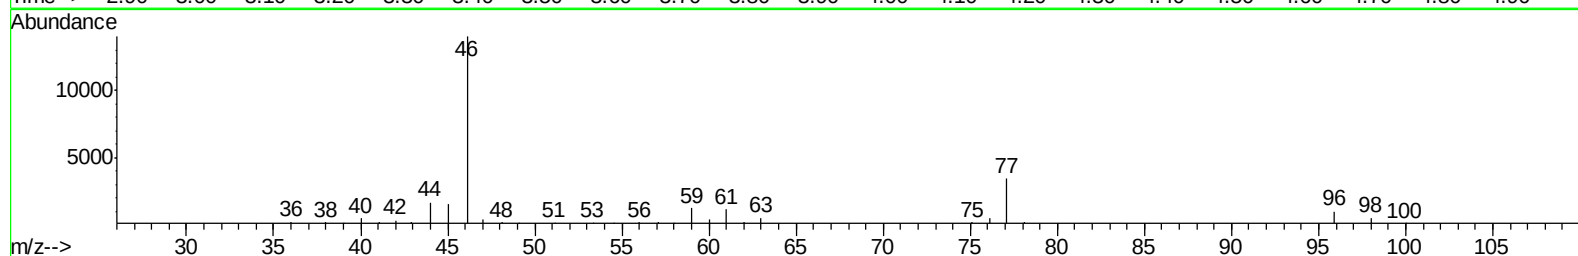


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV100720\
Data File : VV018710.D
Acq On : 06 Oct 2020 23:56
Operator : SY/MD
Sample : L4287-13
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Oct 07 08:22:22 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 07 07:22:30 2020
Response via : Initial Calibration

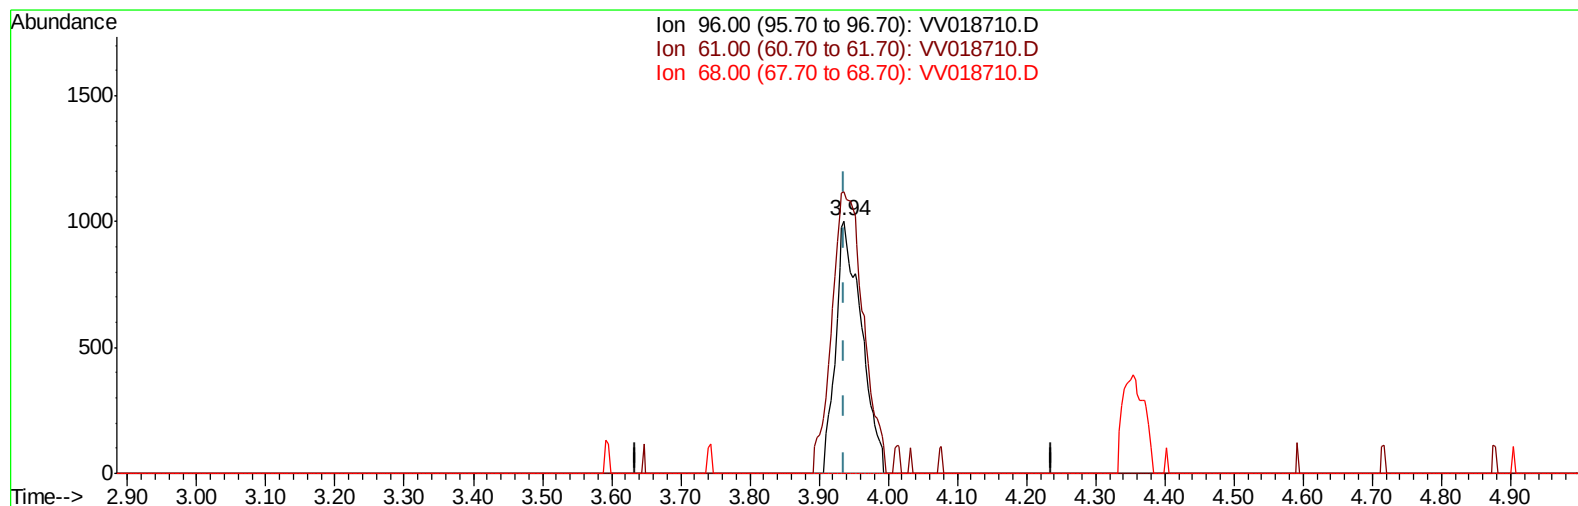

TIC: VV018710.D

(20) cis-1,2-Dichloroethene (T)

3.936min (-0.000) 1.12ug/L m

response 2582

Ion	Exp%	Act%
96.00	100	100
61.00	124.00	111.58
68.00	0.00	0.00
0.00	0.00	0.00