
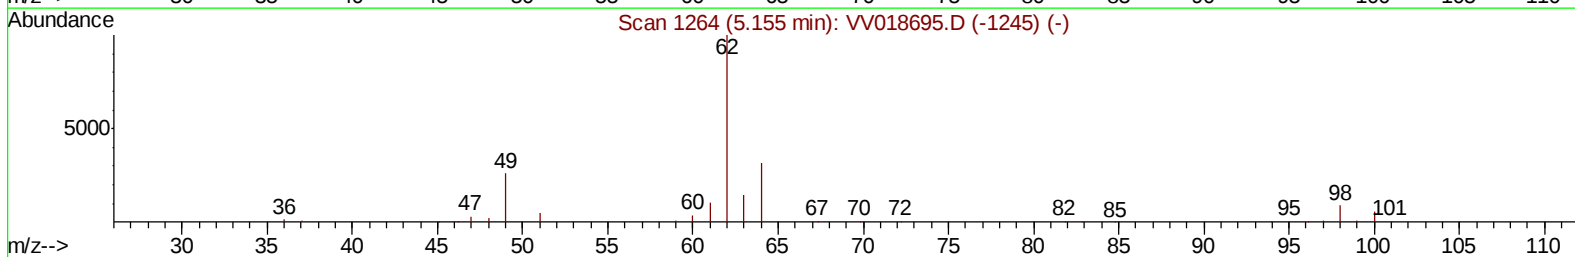
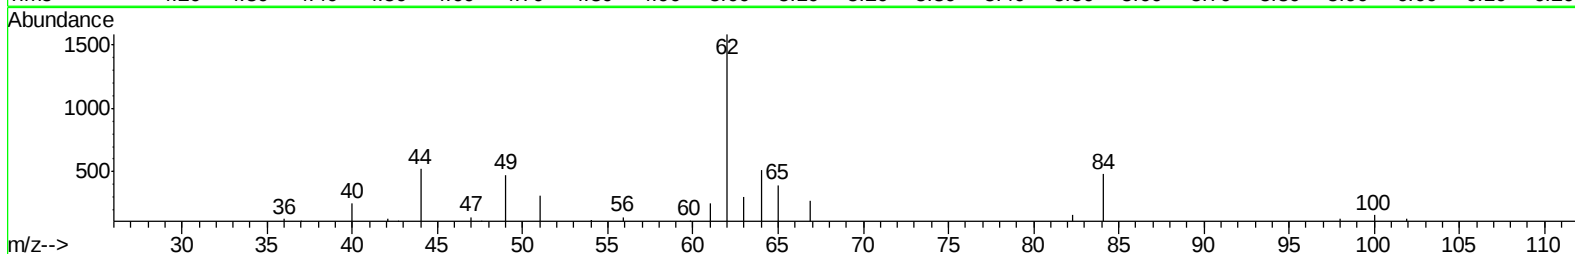


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV100720\
 Data File : VV018710.D
 Acq On : 06 Oct 2020 23:56
 Operator : SY/MD
 Sample : L4287-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Oct 07 08:22:22 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 07 07:22:30 2020
 Response via : Initial Calibration

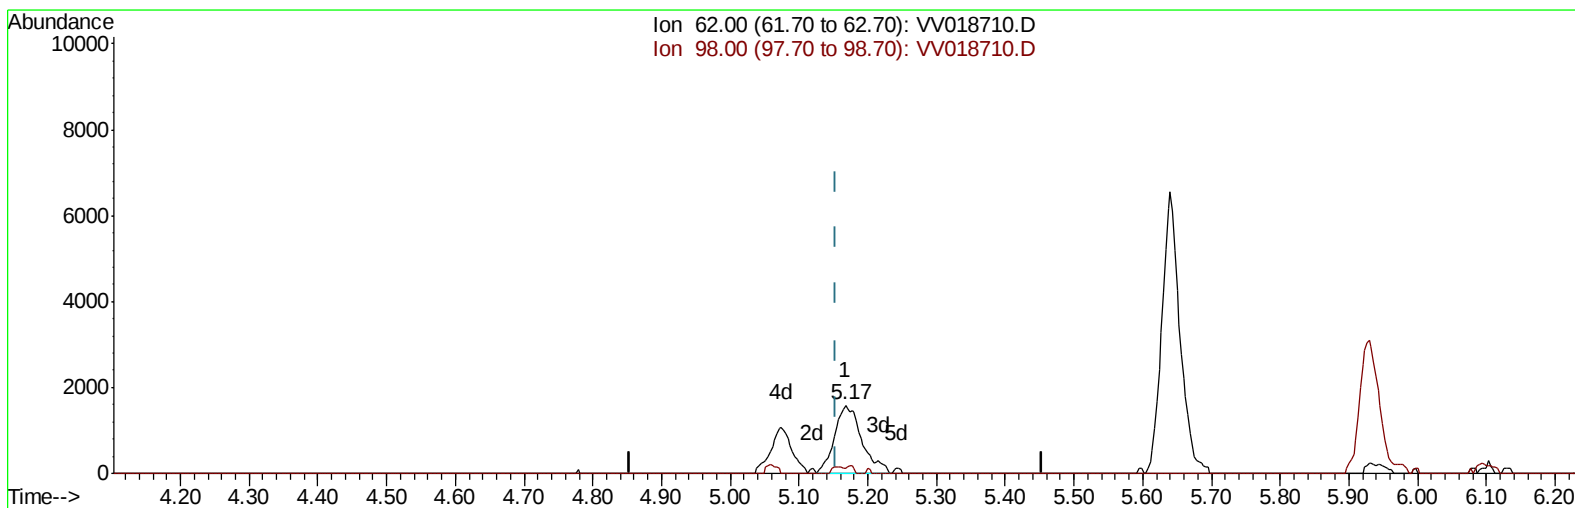

TIC: VV018710.D

(27) 1,2-Dichloroethane (T)

5.167min (+0.013) 1.39ug/L m

response 4356

Ion	Exp%	Act%
62.00	100	100
98.00	9.60	8.53
0.00	0.00	0.00
0.00	0.00	0.00