

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100720\
 Data File : VV018700.D
 Acq On : 06 Oct 2020 20:00
 Operator : SY/MD
 Sample : L4287-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	62	71	96	rBV	5703944	5956717	8.20%	5.219%
2	1.579	145	152	163	rBV	124802	153822	0.21%	0.135%
3	2.126	312	322	344	rVB3	336693	578710	0.80%	0.507%
4	2.672	488	492	495	rVB3	763	603	0.00%	0.001%
5	2.688	495	497	498	rBV2	779	356	0.00%	0.000%
6	2.778	514	525	545	rBV	349593	613438	0.84%	0.537%
7	3.151	638	641	643	rBV2	1167	620	0.00%	0.001%
8	3.357	702	705	708	rVB3	687	411	0.00%	0.000%
9	3.376	708	711	715	rBV3	1054	780	0.00%	0.001%
10	3.576	769	773	775	rBV3	752	530	0.00%	0.000%
11	3.724	816	819	823	rVB2	858	499	0.00%	0.000%
12	3.939	865	886	947	rBV	28285844	72629311	100.00%	63.631%
13	5.071	1222	1238	1266	rBV2	437723	1146287	1.58%	1.004%
14	5.640	1404	1415	1442	rBV	332097	668790	0.92%	0.586%
15	5.936	1491	1507	1537	rBV	3641778	7019728	9.67%	6.150%
16	6.093	1545	1556	1578	rVB	258104	517444	0.71%	0.453%
17	6.418	1656	1657	1662	rBV3	811	565	0.00%	0.000%
18	6.653	1727	1730	1731	rBV2	1008	478	0.00%	0.000%
19	7.007	1829	1840	1863	rBV	143220	262075	0.36%	0.230%
20	7.338	1931	1943	1961	rBV	526895	902146	1.24%	0.790%
21	7.640	2025	2037	2055	rBV3	127952	242061	0.33%	0.212%
22	7.871	2100	2109	2122	rVB9	4734	11244	0.02%	0.010%
23	8.000	2132	2149	2173	rBV	11767322	20073312	27.64%	17.586%
24	8.109	2175	2183	2198	rBV	237087	413752	0.57%	0.362%
25	8.685	2360	2362	2365	rVB3	920	386	0.00%	0.000%
26	8.775	2388	2390	2393	rBV4	892	455	0.00%	0.000%
27	8.871	2408	2420	2444	rBV	515507	840912	1.16%	0.737%
28	9.164	2497	2511	2524	rBV2	14703	27884	0.04%	0.024%
29	9.402	2583	2585	2590	rVB3	641	447	0.00%	0.000%
30	9.463	2600	2604	2607	rBV2	559	490	0.00%	0.000%
31	9.566	2624	2636	2649	rVV2	43378	68640	0.09%	0.060%
32	9.672	2664	2669	2670	rBV3	557	366	0.00%	0.000%
33	9.814	2710	2713	2716	rBV3	675	448	0.00%	0.000%
34	9.875	2729	2732	2736	rVB3	620	453	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100720\
 Data File : VV018700.D
 Acq On : 06 Oct 2020 20:00
 Operator : SY/MD
 Sample : L4287-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

35	9.910	2736	2743	2744	rBV2	383	351	0.00%	0.000%
36	9.926	2744	2748	2750	rBV2	423	317	0.00%	0.000%
37	9.942	2750	2753	2754	rBV3	662	372	0.00%	0.000%
38	9.955	2754	2757	2760	rBV3	1259	1061	0.00%	0.001%
39	10.029	2777	2780	2783	rBV2	567	386	0.00%	0.000%
40	10.071	2791	2793	2795	rVV3	739	313	0.00%	0.000%
41	10.084	2795	2797	2802	rVB4	566	402	0.00%	0.000%
42	10.238	2833	2845	2868	rBV	247977	417588	0.57%	0.366%
43	10.315	2868	2869	2874	rVV3	443	302	0.00%	0.000%
44	10.563	2940	2946	2947	rBV4	1022	983	0.00%	0.001%
45	10.592	2953	2955	2959	rVB2	1186	637	0.00%	0.001%
46	10.649	2968	2973	2975	rBV5	704	629	0.00%	0.001%
47	10.768	3002	3010	3020	rVB10	6530	9879	0.01%	0.009%
48	10.881	3041	3045	3047	rBV4	536	342	0.00%	0.000%
49	10.939	3053	3063	3073	rBV4	7036	10213	0.01%	0.009%
50	11.045	3088	3096	3103	rBV8	4824	7517	0.01%	0.007%
51	11.106	3111	3115	3121	rVB5	1841	2072	0.00%	0.002%
52	11.190	3138	3141	3144	rBV3	1101	715	0.00%	0.001%
53	11.212	3144	3148	3155	rVV7	2538	2738	0.00%	0.002%
54	11.270	3155	3166	3184	rVV	459832	700484	0.96%	0.614%
55	11.360	3189	3194	3206	rVB7	7324	11736	0.02%	0.010%
56	11.646	3272	3283	3296	rBV	474726	739977	1.02%	0.648%
57	11.929	3369	3371	3374	rVV3	815	370	0.00%	0.000%
58	11.968	3375	3383	3388	rVB7	2089	2651	0.00%	0.002%
59	12.084	3417	3419	3424	rVB2	785	480	0.00%	0.000%
60	12.135	3432	3435	3437	rBV2	742	440	0.00%	0.000%
61	12.196	3449	3454	3460	rVB7	3654	3840	0.01%	0.003%
62	12.276	3472	3479	3486	rVB10	2605	3642	0.01%	0.003%
63	12.334	3494	3497	3499	rBV2	1213	668	0.00%	0.001%
64	12.373	3506	3509	3511	rBV2	498	392	0.00%	0.000%
65	12.508	3536	3551	3560	rBV9	9054	16470	0.02%	0.014%
66	12.592	3573	3577	3579	rBV2	382	332	0.00%	0.000%
67	12.707	3607	3613	3618	rVB8	1774	2289	0.00%	0.002%
68	12.743	3621	3624	3626	rBV3	1038	495	0.00%	0.000%
69	12.826	3646	3650	3652	rBV3	608	543	0.00%	0.000%
70	12.871	3656	3664	3666	rBV5	1097	1453	0.00%	0.001%
71	12.903	3669	3674	3675	rBV4	2697	1983	0.00%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100720\
 Data File : VV018700.D
 Acq On : 06 Oct 2020 20:00
 Operator : SY/MD
 Sample : L4287-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

72	12.968	3687	3694	3701	rVB7	3482	4914	0.01%	0.004%
73	13.119	3733	3741	3751	rBV7	2781	5111	0.01%	0.004%
74	13.196	3762	3765	3767	rBV3	1017	591	0.00%	0.001%
75	13.286	3790	3793	3795	rBV4	992	689	0.00%	0.001%
76	13.466	3838	3849	3858	rVB4	12750	24607	0.03%	0.022%
77	13.534	3867	3870	3875	rBV3	1137	808	0.00%	0.001%
78	13.637	3897	3902	3909	rVB5	2681	3219	0.00%	0.003%
79	13.730	3924	3931	3940	rBV4	3058	4589	0.01%	0.004%
80	13.852	3965	3969	3974	rVB3	542	602	0.00%	0.001%
81	13.874	3974	3976	3980	rVB3	583	393	0.00%	0.000%
82	14.003	4014	4016	4019	rBV2	570	379	0.00%	0.000%
83	14.019	4019	4021	4025	rVV2	877	701	0.00%	0.001%
84	14.051	4029	4031	4034	rBV3	562	372	0.00%	0.000%
85	14.067	4034	4036	4040	rVB3	712	468	0.00%	0.000%
86	14.264	4094	4097	4102	rVB2	952	631	0.00%	0.001%
87	14.289	4102	4105	4107	rBV	456	323	0.00%	0.000%
88	14.302	4107	4109	4111	rBV2	661	361	0.00%	0.000%
89	14.363	4122	4128	4131	rBV4	964	928	0.00%	0.001%
90	14.456	4150	4157	4164	rVV7	4931	6939	0.01%	0.006%
91	14.521	4174	4177	4178	rBV7	560	295	0.00%	0.000%
92	14.569	4190	4192	4194	rVB2	804	323	0.00%	0.000%
93	14.630	4208	4211	4212	rBV2	607	301	0.00%	0.000%
94	14.714	4232	4237	4240	rBV5	919	861	0.00%	0.001%
95	14.900	4293	4295	4298	rVB2	812	362	0.00%	0.000%
96	15.180	4379	4382	4386	rVB4	753	601	0.00%	0.001%
97	15.382	4440	4445	4449	rBV4	1000	1014	0.00%	0.001%
98	15.408	4451	4453	4456	rVV2	672	295	0.00%	0.000%
99	15.456	4465	4468	4472	rBV2	608	426	0.00%	0.000%
100	15.968	4625	4627	4629	rBV2	644	319	0.00%	0.000%


Sum of corrected areas: 114140644

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100720\
Data File : VV018700.D
Acq On : 06 Oct 2020 20:00
Operator : SY/MD
Sample : L4287-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

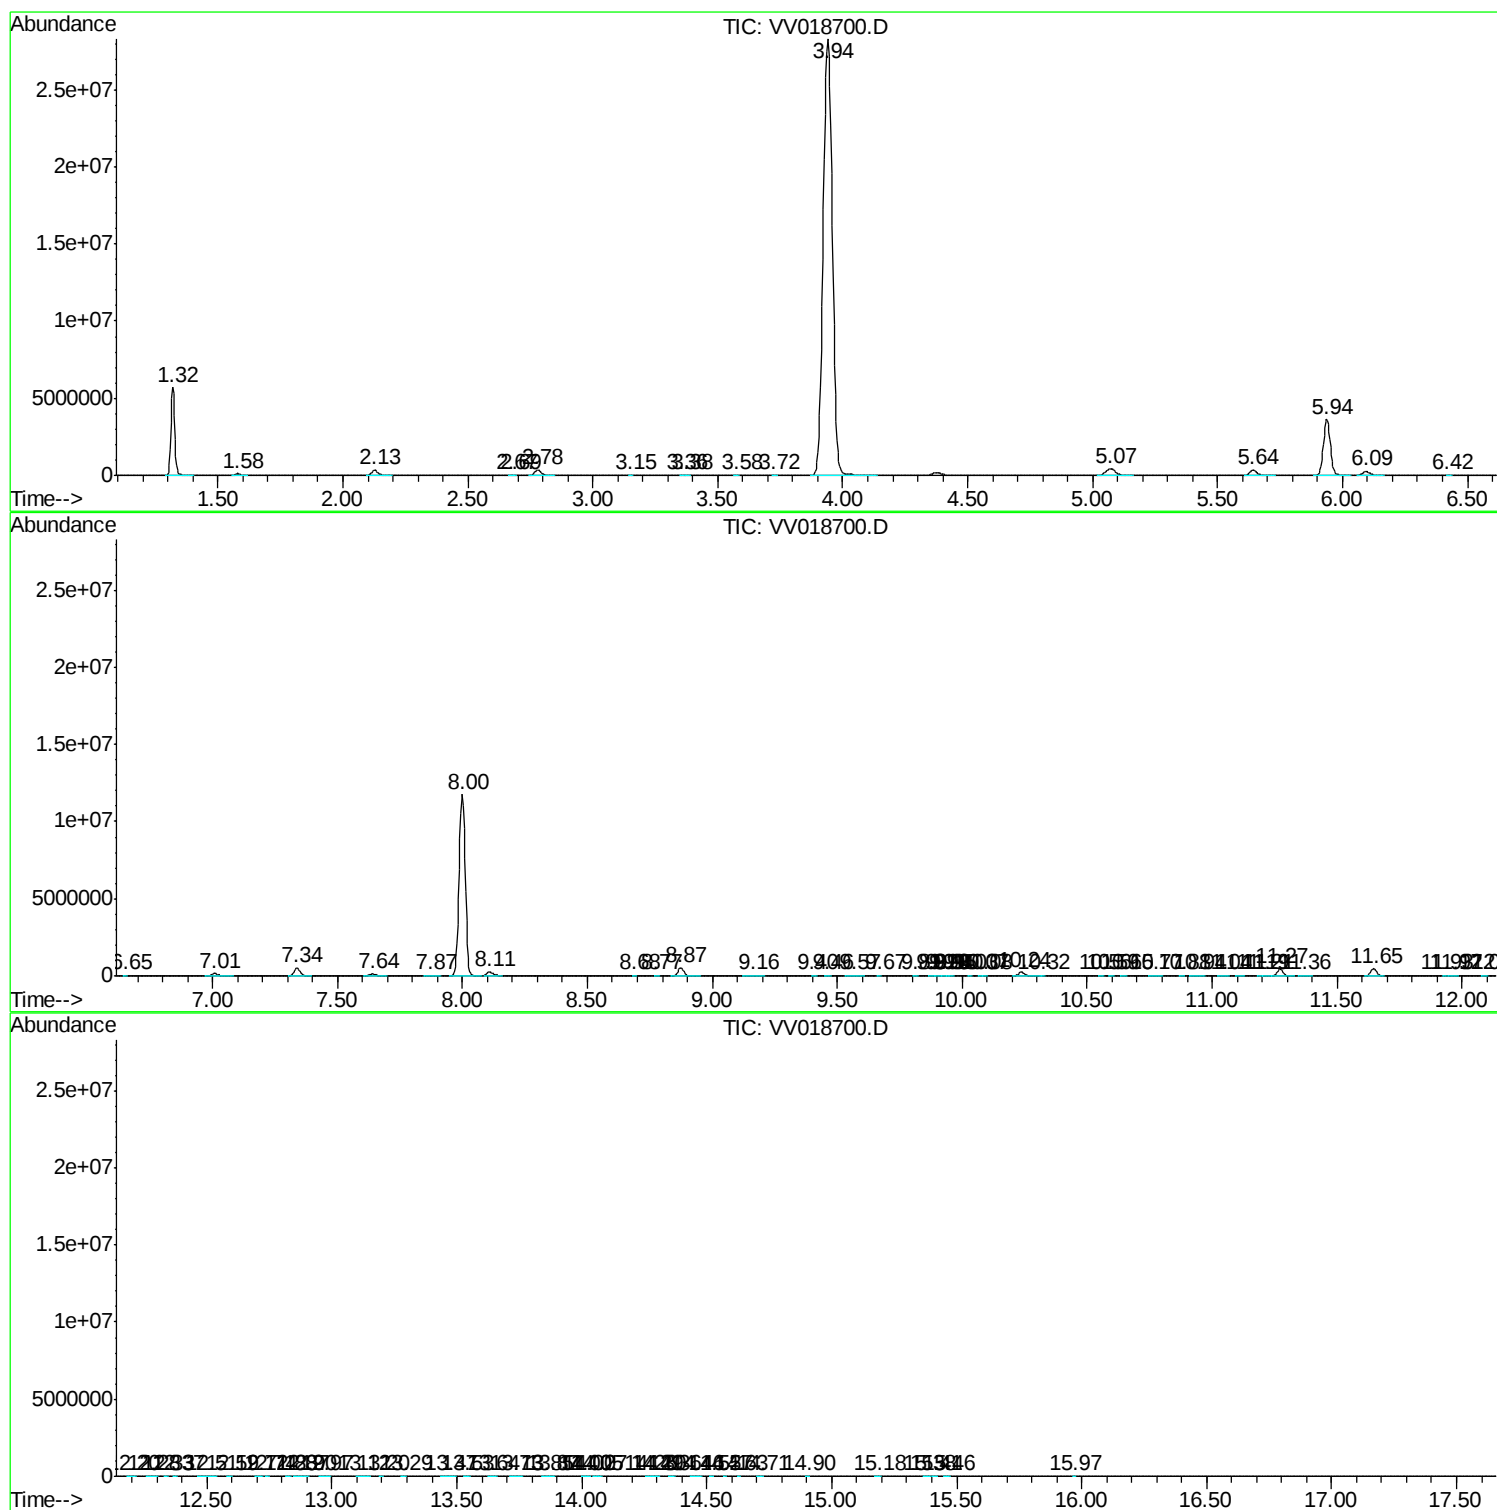

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV100720\
Data File : VV018700.D
Acq On : 06 Oct 2020 20:00
Operator : SY/MD
Sample : L4287-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV100720\
Data File : VV018700.D
Acq On : 06 Oct 2020 20:00
Operator : SY/MD
Sample : L4287-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc