

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100720\
 Data File : VV018717.D
 Acq On : 07 Oct 2020 02:43
 Operator : SY/MD
 Sample : L4287-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	82	rVB2	146480	155463	16.90%	2.000%
2	1.576	145	151	162	rVB	112472	122846	13.35%	1.581%
3	2.119	312	320	340	rVB	230550	345375	37.54%	4.444%
4	2.412	409	411	414	rBV	705	445	0.05%	0.006%
5	2.515	440	443	445	rBV3	652	479	0.05%	0.006%
6	2.586	461	465	467	rBV2	598	458	0.05%	0.006%
7	2.608	470	472	479	rVV4	932	672	0.07%	0.009%
8	2.656	485	487	493	rVV4	670	498	0.05%	0.006%
9	2.782	515	526	539	rBV3	9034	18064	1.96%	0.232%
10	2.936	572	574	578	rVB2	592	371	0.04%	0.005%
11	2.997	591	593	596	rVB	842	372	0.04%	0.005%
12	3.029	599	603	607	rBV3	915	691	0.08%	0.009%
13	3.061	608	613	615	rBV5	1129	1167	0.13%	0.015%
14	3.203	654	657	659	rBV2	733	447	0.05%	0.006%
15	3.267	674	677	678	rBV2	752	385	0.04%	0.005%
16	3.312	687	691	696	rVB3	729	520	0.06%	0.007%
17	3.348	698	702	705	rBV3	582	399	0.04%	0.005%
18	3.422	722	725	728	rVB	576	351	0.04%	0.005%
19	3.557	763	767	770	rBV	444	361	0.04%	0.005%
20	3.650	791	796	798	rBV3	407	374	0.04%	0.005%
21	3.682	804	806	809	rBV2	704	438	0.05%	0.006%
22	3.775	831	835	836	rBV3	966	718	0.08%	0.009%
23	3.843	854	856	861	rVB2	796	593	0.06%	0.008%
24	3.872	861	865	866	rBV2	818	436	0.05%	0.006%
25	3.933	866	884	907	rBV2	95101	358918	39.01%	4.618%
26	4.238	976	979	981	rBV3	624	380	0.04%	0.005%
27	4.373	1004	1021	1049	rBV2	149899	375463	40.81%	4.831%
28	4.608	1093	1094	1099	rVB	654	358	0.04%	0.005%
29	4.656	1106	1109	1113	rBV3	612	510	0.06%	0.007%
30	4.881	1174	1179	1184	rBV6	847	1017	0.11%	0.013%
31	4.975	1204	1208	1210	rBV2	531	451	0.05%	0.006%
32	5.071	1221	1238	1260	rBV2	357941	920034	100.00%	11.837%
33	5.367	1327	1330	1334	rBV2	1081	933	0.10%	0.012%
34	5.531	1378	1381	1382	rBV3	905	409	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100720\
 Data File : VV018717.D
 Acq On : 07 Oct 2020 02:43
 Operator : SY/MD
 Sample : L4287-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

35	5.582	1393	1397	1399	rBV3	532	443	0.05%	0.006%
36	5.640	1403	1415	1439	rBV	332099	658754	71.60%	8.476%
37	5.933	1493	1506	1525	rBV6	29653	70762	7.69%	0.910%
38	6.093	1543	1556	1580	rBV2	213371	442147	48.06%	5.689%
39	6.354	1634	1637	1639	rBV3	803	577	0.06%	0.007%
40	6.466	1668	1672	1674	rBV3	603	503	0.05%	0.006%
41	6.550	1693	1698	1701	rBV4	1213	1173	0.13%	0.015%
42	6.849	1789	1791	1794	rBV2	565	378	0.04%	0.005%
43	6.913	1807	1811	1815	rBV3	1006	928	0.10%	0.012%
44	7.007	1829	1840	1862	rBV2	123030	225049	24.46%	2.895%
45	7.338	1932	1943	1961	rBV	475673	805982	87.60%	10.370%
46	7.643	2028	2038	2054	rBV	82418	141015	15.33%	1.814%
47	7.843	2097	2100	2103	rBV2	779	631	0.07%	0.008%
48	7.904	2114	2119	2124	rVB3	575	517	0.06%	0.007%
49	7.933	2124	2128	2131	rBV2	684	473	0.05%	0.006%
50	7.997	2138	2148	2160	rBV3	18664	32894	3.58%	0.423%
51	8.106	2173	2182	2215	rBV2	179980	387112	42.08%	4.981%
52	8.408	2274	2276	2281	rVB5	597	380	0.04%	0.005%
53	8.601	2332	2336	2338	rBV2	815	591	0.06%	0.008%
54	8.685	2360	2362	2367	rVB4	809	538	0.06%	0.007%
55	8.833	2404	2408	2409	rBV3	665	446	0.05%	0.006%
56	8.871	2409	2420	2438	rVV	511966	824004	89.56%	10.602%
57	9.126	2497	2499	2502	rBV3	614	397	0.04%	0.005%
58	9.222	2524	2529	2531	rBV3	711	576	0.06%	0.007%
59	9.293	2550	2551	2555	rVB	734	386	0.04%	0.005%
60	9.312	2555	2557	2561	rBV2	712	575	0.06%	0.007%
61	9.434	2593	2595	2601	rVB5	571	444	0.05%	0.006%
62	9.498	2611	2615	2618	rBV2	619	554	0.06%	0.007%
63	9.566	2632	2636	2637	rBV2	703	502	0.05%	0.006%
64	9.765	2696	2698	2700	rVB	885	378	0.04%	0.005%
65	9.785	2701	2704	2707	rVB	609	356	0.04%	0.005%
66	9.804	2707	2710	2711	rBV2	745	358	0.04%	0.005%
67	9.871	2730	2731	2736	rBV2	701	453	0.05%	0.006%
68	10.238	2833	2845	2863	rBV	250202	395715	43.01%	5.091%
69	10.354	2880	2881	2887	rVB2	547	424	0.05%	0.005%
70	10.531	2934	2936	2940	rVB2	603	405	0.04%	0.005%
71	10.624	2961	2965	2968	rBV3	981	711	0.08%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100720\
 Data File : VV018717.D
 Acq On : 07 Oct 2020 02:43
 Operator : SY/MD
 Sample : L4287-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

72	10.643	2968	2971	2977	rVB4	526	519	0.06%	0.007%
73	10.707	2988	2991	2997	rVB4	564	519	0.06%	0.007%
74	10.743	2997	3002	3004	rBV	629	550	0.06%	0.007%
75	10.897	3046	3050	3052	rBV2	496	435	0.05%	0.006%
76	10.945	3061	3065	3069	rVB2	1119	778	0.08%	0.010%
77	11.074	3101	3105	3106	rBV2	467	358	0.04%	0.005%
78	11.129	3118	3122	3125	rBV2	434	356	0.04%	0.005%
79	11.193	3140	3142	3145	rVB2	926	532	0.06%	0.007%
80	11.270	3152	3166	3184	rBV	491134	753970	81.95%	9.701%
81	11.379	3198	3200	3205	rBV2	981	637	0.07%	0.008%
82	11.550	3250	3253	3255	rBV3	678	356	0.04%	0.005%
83	11.579	3258	3262	3266	rBV4	1143	950	0.10%	0.012%
84	11.646	3271	3283	3300	rBV	441599	696856	75.74%	8.966%
85	11.810	3330	3334	3335	rBV3	547	378	0.04%	0.005%
86	11.961	3377	3381	3383	rBV	538	422	0.05%	0.005%
87	12.074	3414	3416	3422	rVB3	649	400	0.04%	0.005%
88	12.473	3534	3540	3542	rBV2	576	436	0.05%	0.006%
89	12.569	3566	3570	3571	rBV3	735	406	0.04%	0.005%
90	12.678	3602	3604	3608	rVB3	714	358	0.04%	0.005%
91	12.826	3646	3650	3652	rBV3	554	492	0.05%	0.006%
92	13.203	3763	3767	3769	rBV	537	391	0.04%	0.005%
93	13.778	3939	3946	3947	rBV2	744	570	0.06%	0.007%
94	13.961	4000	4003	4006	rBV2	574	424	0.05%	0.005%
95	14.260	4093	4096	4103	rVB4	762	696	0.08%	0.009%
96	14.556	4185	4188	4191	rBV2	1026	615	0.07%	0.008%
97	14.588	4195	4198	4202	rVV3	730	548	0.06%	0.007%
98	14.765	4250	4253	4257	rBV3	562	396	0.04%	0.005%
99	14.807	4261	4266	4268	rBV2	670	640	0.07%	0.008%
100	15.141	4365	4370	4371	rBV3	586	492	0.05%	0.006%


Sum of corrected areas: 7772407

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100720\
Data File : VV018717.D
Acq On : 07 Oct 2020 02:43
Operator : SY/MD
Sample : L4287-20
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

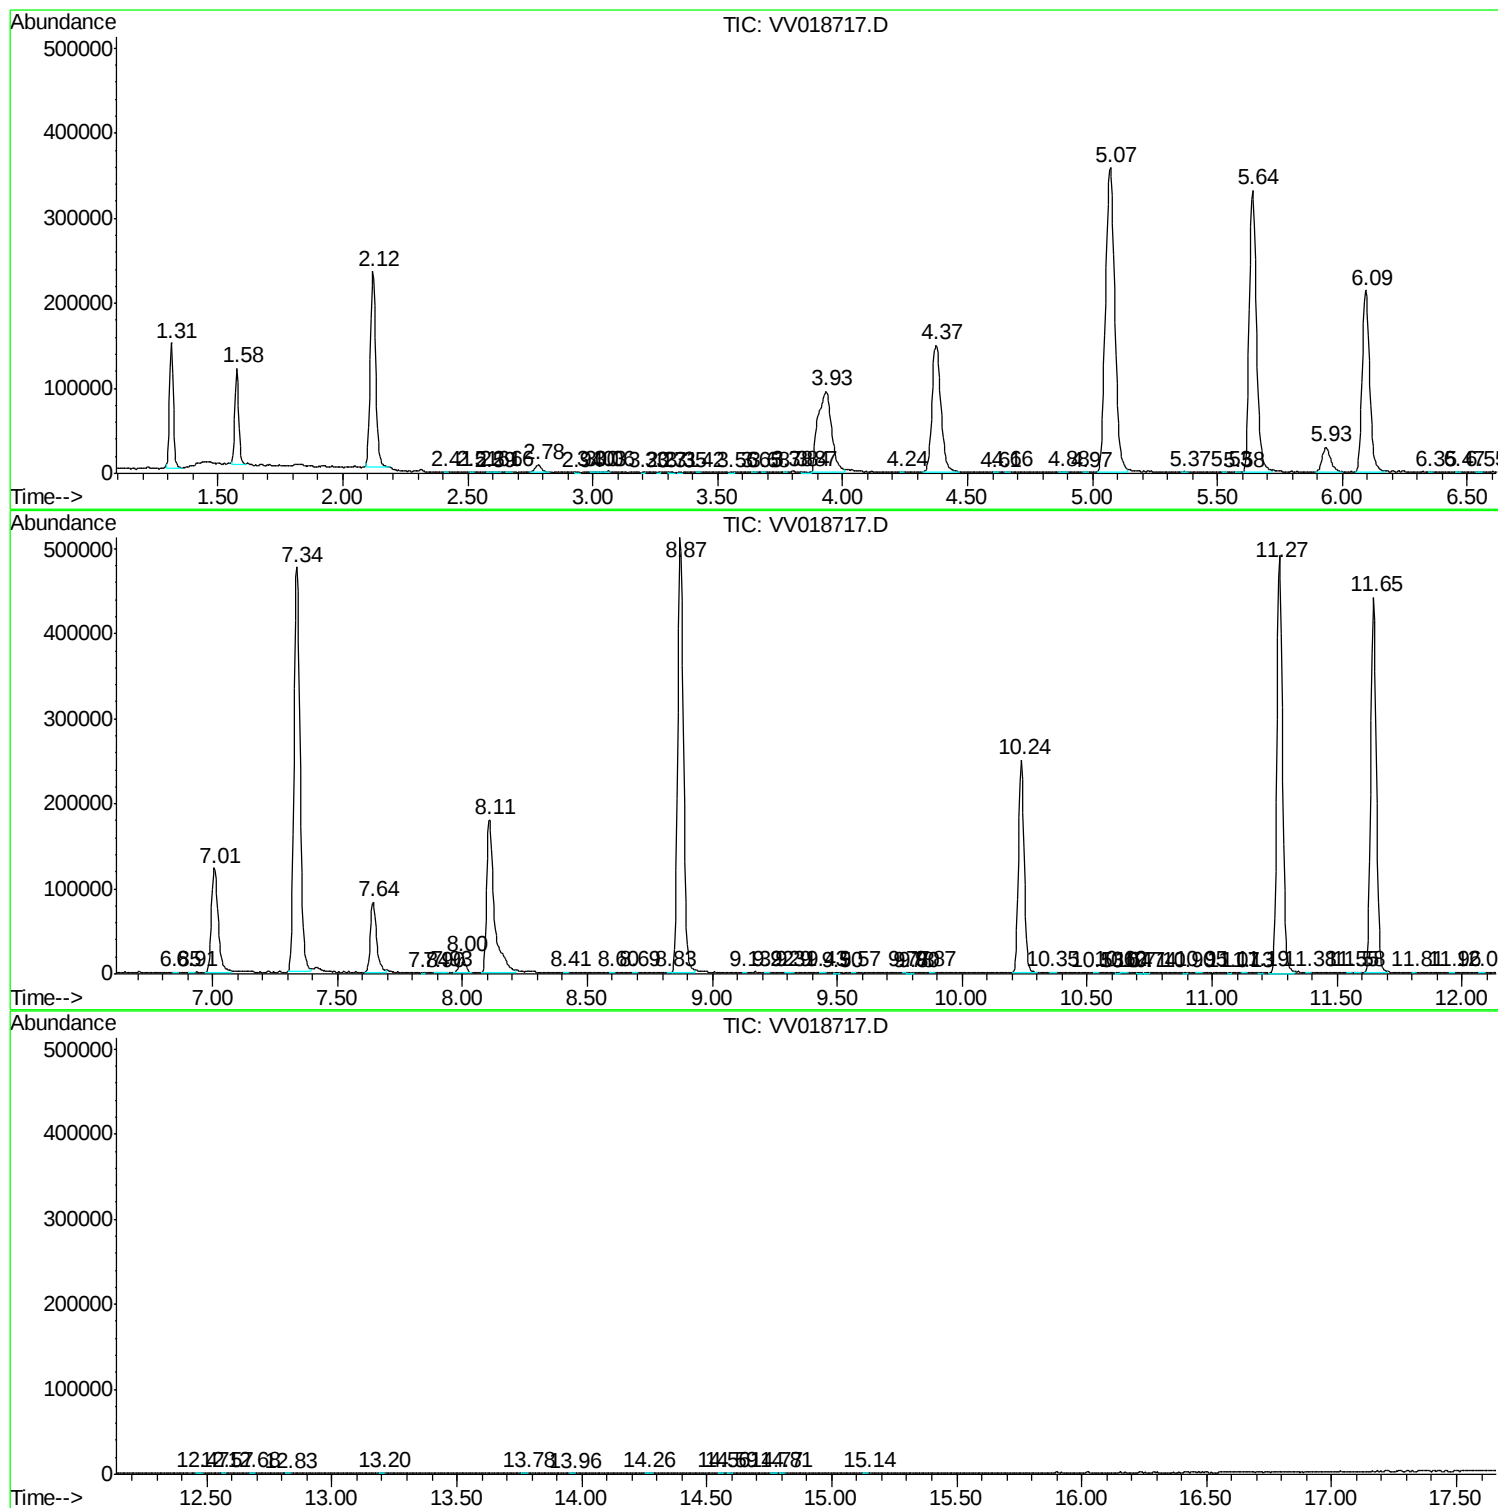

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV100720\
Data File : VV018717.D
Acq On : 07 Oct 2020 02:43
Operator : SY/MD
Sample : L4287-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV100720\
Data File : VV018717.D
Acq On : 07 Oct 2020 02:43
Operator : SY/MD
Sample : L4287-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc